Medicina **P1000** Enteral Syringe Pump

Quick Start Guide

Turn pump on

Press ⏻ to activate and turn on the pump,
the pump will run start-up checks and display the start-up screen.

Install syringe

The system will inspect whether the syringe is installed after completing the self-test.

Confirm syringe

On the [Confirm Syringe] screen, if an ENFit enteral syringe is installed, press OK to confirm; if other syringe is installed, press Clear you will be warned with **[Danger! Enteral syringe not chosen!]**.

Priming the line

On the infusion parameters setting interface, press Bolus to enter [Priming] prompt screen. Hold down Bolus to prime the line, release after air bubbles are removed.

⚠ During the purge, please disconnect the pump from the patient.

Set infusion parameters

Select volume, rate or time using the OK button and set the parameter using the arrows. Select OK to confirm. Volume, rate and time are independent. The third will be calculated automatically.

Connect to patient

Start Infusion

Press Start Press and hold Menu to lock parameters. Alternatively select [Main Menu] ➔ [General Option] ➔ [Auto-lock time] to set automatic locking function. To unlock parameter screen, press and hold Menu

Press Stop

Finish

A 'near end alarm' can be set 1-30 minutes from the end of infusion [Main Menu] ➔ [General Option] ➔ [Time near end]. Press SILENCE to mute. When the infusion is finished an alarm will sound. Press STOP.

Remove syringe

Disconnect from the patient and remove the syringe in a correct manner.

Turn pump off

Hold down ⏻ until the Power Off progress bar completes.

medicina

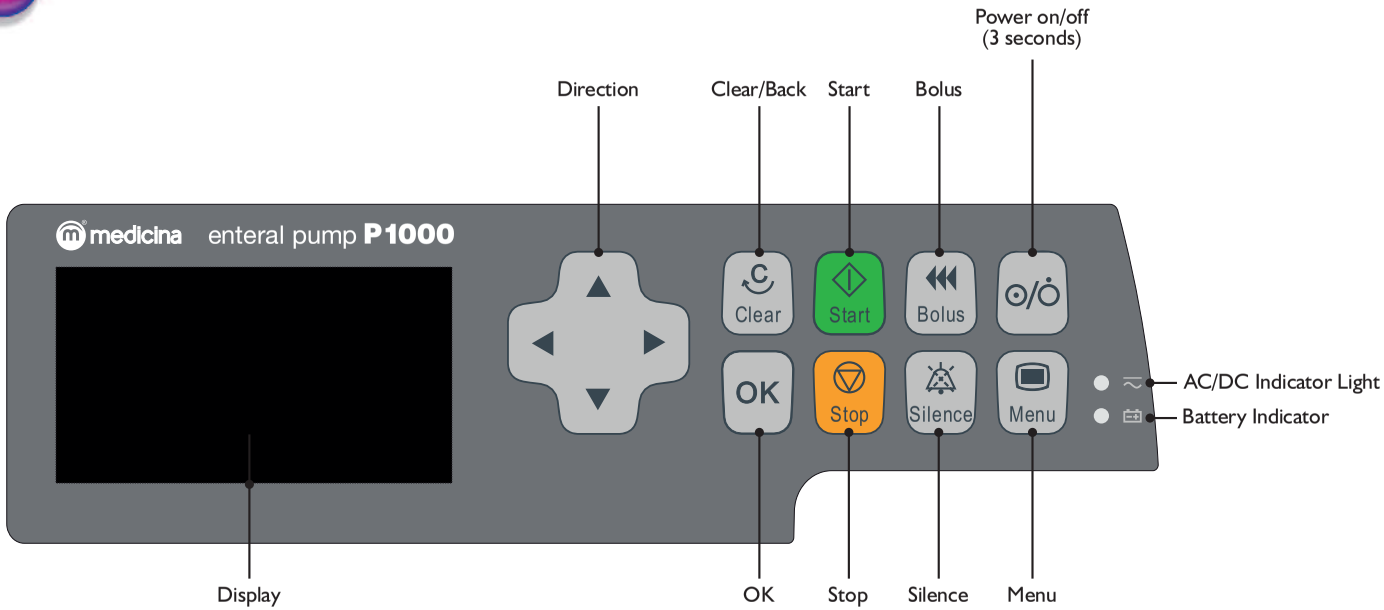

amsl medical

2 McCabe Place
Chatswood NSW
Australia 2067

P 02 9882 3666
E amsl@amsl.com.au
W www.amsl.com.au

PR-100-122