



New SuperLine II
Product Catalog

Dentium
For Dentists By Dentists

Contents

| | | |
|--------------------------------------|---|--|
| New SuperLine II | Characteristics | 06 |
| | Color Coding by Diameter | 07 |
| | Fixture | 08 |
| Surgical Components | Cover Screw | 09 |
| | GBR Healing Abutment | 09 |
| | Healing Abutment | 10 |
| | Scan Abutment | 12 |
| Prosthetic Procedure 1 | Dual / Combi Abutment - Abutment Level Impression | 13 |
| | Combi Abutment | 14 |
| | Dual Abutment | 15 |
| | Abutment Level Impression Components | 17 |
| | Restorative Kit | 18 |
| Prosthetic Procedure 2 | Dual / Custom / Milling / Angled / Direct-Casting / Metal-Casting / Temporary (Plastic & Ti) Abutment - Fixture Level Impression | 19 |
| | Fixture Level Impression Components | 20 |
| | Milling Abutment | 22 |
| | Angled Abutment | 24 |
| | Direct-Casting Abutment | 26 |
| | Metal-Casting Abutment | 26 |
| | Ti-Temporary Abutment | 27 |
| | Plastic Temporary Abutment | 27 |
| | Prosthetic Procedure 3 | Screw Abutment - Abutment Level Impression |
| Screw Abutment | | 29 |
| Angled Screw Abutment | | 30 |
| Screw Abutment Impression Components | | 31 |
| Prosthetic Procedure 4 | Overdenture Procedure - Positioner / Mini Ball / Magnetic Attachment | 34 |
| | Positioner | 35 |
| | Mini Ball Attachment | 37 |
| | Magnetic Attachment | 38 |

Instruments

| | |
|--|----|
| Surgical Kit (Full) | 40 |
| Surgical Kit (Stopper Drill Full) | 41 |
| Surgical Kit (Standard) | 42 |
| Surgical Kit (Short Implant) | 43 |
| Surgical Kit (Stopper Drill Kit) | 44 |
| Surgical Kit (Drill Stopper Kit) | 45 |
| Surgical Instrument | 46 |
| Osteotome Kit | 55 |
| Trephine Kit | 56 |
| Instrument | 57 |
| Screws& Pins | 58 |
| Prosthetic Kit | 59 |
| Planning Kit | 60 |
| Prosthetic and Laboratory Instrument | 61 |
| Help Kit | 62 |
| Polymer Guide Kit | 63 |
| DASK | 64 |
| Sinus Bur Kit | 65 |
| DASK / Sinus Bur Kit | 66 |
| Ridge Spreader Kit | 67 |
| Sinus Kit | 68 |
| Ridge Expander Kit | 69 |
| Implant Guide Kit | 70 |
| Digital Guide I Simple Kit I Positioning, Anchor | 71 |
| Digital Guide I Full Kit I FX 36/40/45 | 72 |
| Digital Guide I 5.0 Kit I FX 36/40/45/50 | 73 |



S.L.A. Surface

S.L.A. (Sandblasting with Large grits and Acid etching)

- Higher bone-to-implant contact
- Faster bone formation on the surface

reference: Kim H., et. al. "The Biocompatibility of SLA-treated Titanium Implants" Biomed. Mater. 2008; 3(2):025011

In vivo test




SuperLine

New SuperLine II Characteristics

Joint stability & Improved strength for zirconia crown

- Abutment material: Grade 4 ➔ Ti-6Al-4V ELI

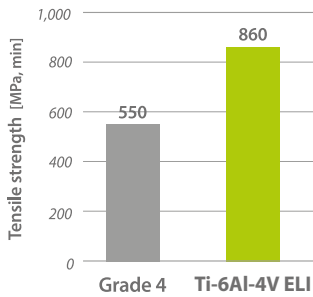


- Long hex design: Improved recognition

Improved soft tissue management

- Concave abutment design

Improved wall thickness



Double thread & Tapered design




Double threaded tapered body design may provide better success rate in immediate loading cases.









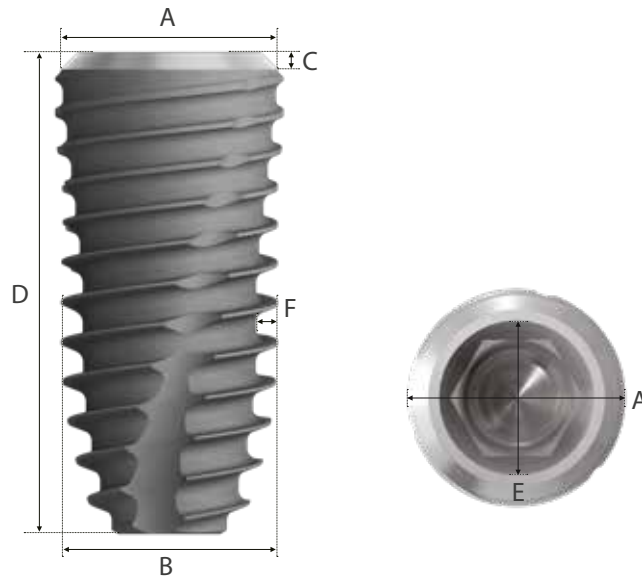



reference: Kim et. al., "A Prospective, 1-year observational study of double-threaded tapered body dental implants with immediate loading" J Prosthet Dent 2015;114:46-51

Height and sharper thread design



New SuperLine II Fixture Specifications




| Fixture (Mount Free) | |  |  |  |  |  |  | |
|----------------------|-----------------------|---|---|---|--|---|---|------|
| A | Platform Diameter(Ø) | 3.6 | 4.0 | 4.5 | 5.0 | 6.0 | 7.0 | |
| B | Body Diameter(Ø) | 3.6 | 4.0 | 4.5 | 5.0 | 5.0 | 5.8 | |
| C | Bevel Height (mm) | L: 7 | 1.5 | 1.5 | 1.5 | 1.5 | 1.5 | 1.5 |
| | | L: 8, 10, 12, 14 | 0.03 | 0.20 | 0.35 | 0.60 | 0.70 | 1.00 |
| D | Total Length(mm) | 7, 8, 10, 12, 14 | | | | | | |
| E | Abutment Interface(Ø) | 3.33 | 3.33 | 3.33 | 3.33 | 3.33 | 3.33 | |
| F | Thread Depth(mm) | 0.38 | 0.40 | 0.45 | 0.50 | 0.50 | 0.50 | |
| Cap Color | |  |  |  |  |  |  | |
| | | Yellow | Green | Blue | Red | Orange | Violet | |
| Selection Guideline | | Anterior | Anterior | Premolar | Molar | Molar | Molar | |

New SuperLine II Fixture


Unit: mm, Scale 1.5 : 1

· Cover screw is not included in the package


| Platform | Body | L | Art. No. |
|----------|-------|----|-----------|
| Ø 3.7 | Ø 3.6 | 7 | FXS 36 07 |
| | | 8 | FXS 36 08 |
| | | 10 | FXS 36 10 |
| | | 12 | FXS 36 12 |
| | | 14 | FXS 36 14 |

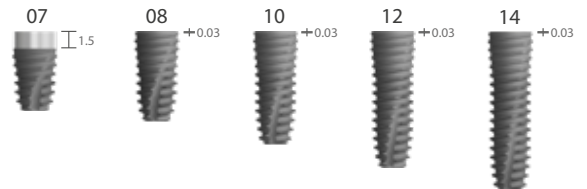


| | | | |
|-------|-------|----|-----------|
| Ø 4.0 | Ø 4.0 | 7 | FXS 40 07 |
| | | 8 | FXS 40 08 |
| | | 10 | FXS 40 10 |
| | | 12 | FXS 40 12 |
| | | 14 | FXS 40 14 |

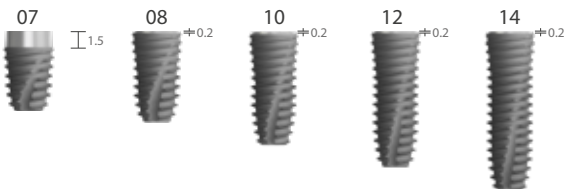


| | | | |
|-------|-------|----|-----------|
| Ø 4.5 | Ø 4.5 | 7 | FXS 45 07 |
| | | 8 | FXS 45 08 |
| | | 10 | FXS 45 10 |
| | | 12 | FXS 45 12 |
| | | 14 | FXS 45 14 |

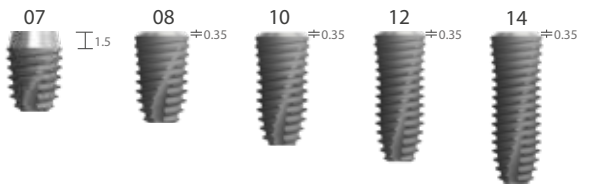


| | | | |
|-------|-------|----|-----------|
| Ø 5.0 | Ø 5.0 | 7 | FXS 50 07 |
| | | 8 | FXS 50 08 |
| | | 10 | FXS 50 10 |
| | | 12 | FXS 50 12 |
| | | 14 | FXS 50 14 |

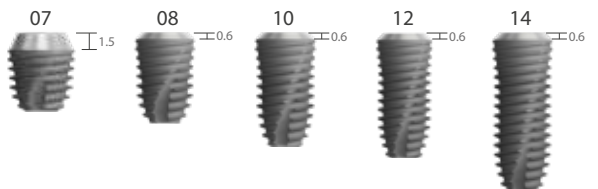

| | | | |
|-------|-------|----|-----------|
| Ø 6.0 | Ø 5.0 | 7 | FXS 60 07 |
| | | 8 | FXS 60 08 |
| | | 10 | FXS 60 10 |
| | | 12 | FXS 60 12 |
| | | 14 | FXS 60 14 |

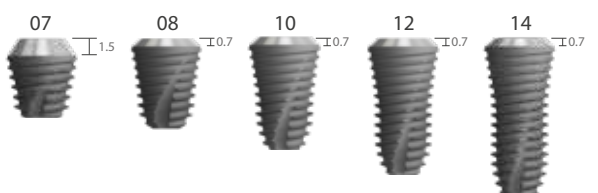

| | | | |
|-------|-------|----|-----------|
| Ø 7.0 | Ø 5.8 | 7 | FXS 70 07 |
| | | 8 | FXS 70 08 |
| | | 10 | FXS 70 10 |
| | | 12 | FXS 70 12 |
| | | 14 | FXS 70 14 |

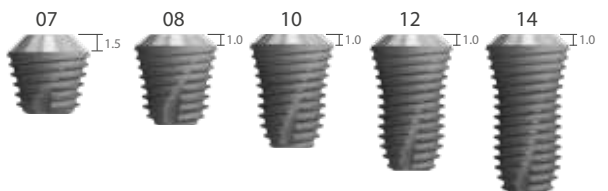

※ Note: To prevent damage to the Implant driver or fixture, do not over torque during fixture insertion.


Cover Screw

Unit: mm, Scale 1.5 : 1

• Single use only




| Color | Diameter | Art. No. |
|-------|-------------------|----------|
| Green | \varnothing 3.6 | CS 36 |



※ Hex driver: Use no more than 5N-cm of torque when screwing Cover Screw to a fixture.
If hex is worn, slot on the head of the product can be used to rotate it.

GBR Healing Abutment

Unit: mm, Scale 1.5 : 1

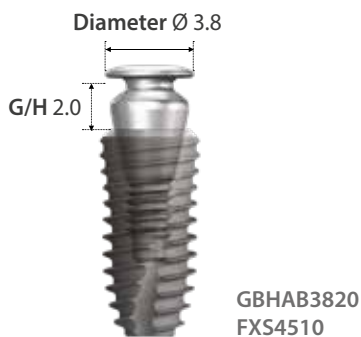

| Diameter | G/H | Art. No. |
|-------------------|-----|-------------|
| \varnothing 3.3 | 3.5 | GBHAB 33 35 |
| \varnothing 3.8 | 0.5 | GBHAB 38 05 |
| \varnothing 3.8 | 2.0 | GBHAB 38 20 |



※ Hex driver: Use no more than 10N-cm of torque when screwing GBR Healing Abutment to a fixture.
If hex is worn, slot on the head of the product can be used to rotate it.


Healing Abutment

Unit: mm, Scale 1.5 : 1

• Single use only



| Diameter | G/H | H | Art. No. |
|----------|-----|-----|----------------|
| Ø 4.0 | 2.0 | 2.0 | HAB 40 20 20 E |
| | 2.0 | 3.5 | HAB 40 20 35 E |
| | 3.0 | 5.0 | HAB 40 30 50 E |
| | 4.0 | 7.0 | HAB 40 40 70 E |
| Ø 4.5 | 2.0 | 2.0 | HAB 45 20 20 E |
| | 2.0 | 3.5 | HAB 45 20 35 E |
| | 3.0 | 5.0 | HAB 45 30 50 E |
| | 4.0 | 7.0 | HAB 45 40 70 E |
| Ø 5.5 | 2.0 | 2.0 | HAB 55 20 20 E |
| | 2.0 | 3.5 | HAB 55 20 35 E |
| | 3.0 | 5.0 | HAB 55 30 50 E |
| | 4.0 | 7.0 | HAB 55 40 70 E |
| Ø 6.5 | 2.0 | 2.0 | HAB 65 20 20 E |
| | 2.0 | 3.5 | HAB 65 20 35 E |
| | 3.0 | 5.0 | HAB 65 30 50 E |
| | 4.0 | 7.0 | HAB 65 40 70 E |

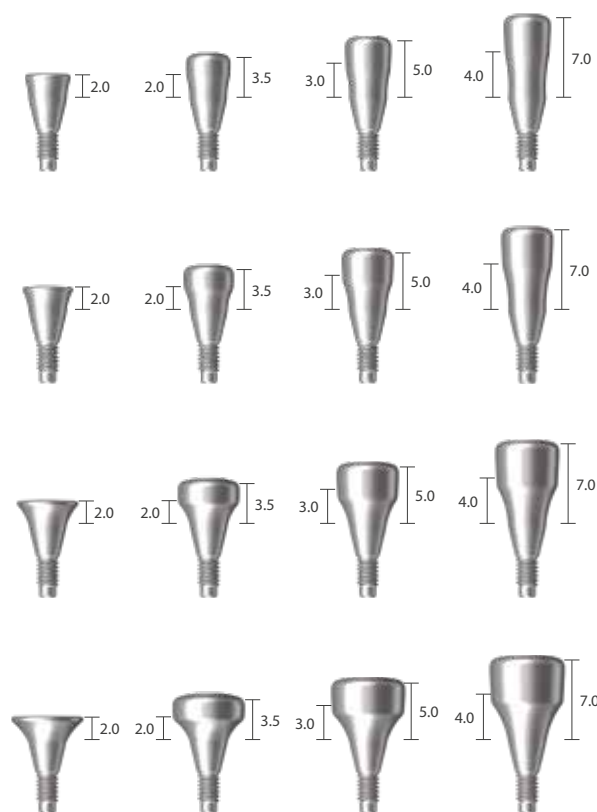


※ Hex driver: Use no more than 10N-cm of torque when screwing Healing Abutment to a fixture.
If hex is worn, slot on the head of the product can be used to rotate it.


Healing Abutment

Unit: mm, Scale 1.5 : 1


| Diameter | G/H | H | Art. No. |
|----------|-----|-----|----------------|
| Ø 7.5 | 2.0 | 3.5 | HAB 75 20 35 E |
| | 3.0 | 5.0 | HAB 75 30 50 E |



| | | | |
|-------|-----|-----|----------------|
| Ø 8.5 | 2.0 | 3.5 | HAB 85 20 35 E |
| | 3.0 | 5.0 | HAB 85 30 50 E |

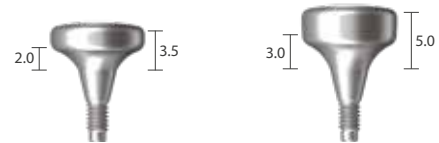

| | | | |
|-------|-----|-----|----------------|
| Ø 9.5 | 2.0 | 3.5 | HAB 95 20 35 E |
| | 3.0 | 5.0 | HAB 95 30 50 E |




※ Hex driver: Use no more than 10N-cm of torque when screwing Healing Abutment to a fixture.
If hex is worn, slot on the head of the product can be used to rotate it.

Scan Abutment


Unit: mm, Scale 1.5 : 1

• Single use only


| Diameter | G/H | H | Type | Art. No. |
|----------|-----|------|---------|--------------|
| Ø 4.0 | 2.5 | 6.0 | Hex | IHAB 40 06 H |
| | 2.5 | 6.0 | Non-hex | IHAB 40 06 N |
| | 3.0 | 8.0 | Hex | IHAB 40 08 H |
| | 3.0 | 8.0 | Non-hex | IHAB 40 08 N |
| | 3.5 | 10.0 | Hex | IHAB 40 10 H |
| | 3.5 | 10.0 | Non-hex | IHAB 40 10 N |

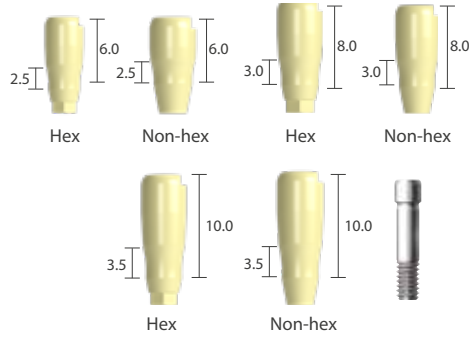

| Diameter | G/H | H | Type | Art. No. |
|----------|-----|------|---------|--------------|
| Ø 5.0 | 2.5 | 6.0 | Hex | IHAB 50 06 H |
| | 2.5 | 6.0 | Non-hex | IHAB 50 06 N |
| | 3.0 | 8.0 | Hex | IHAB 50 08 H |
| | 3.0 | 8.0 | Non-hex | IHAB 50 08 N |
| | 3.5 | 10.0 | Hex | IHAB 50 10 H |
| | 3.5 | 10.0 | Non-hex | IHAB 50 10 N |

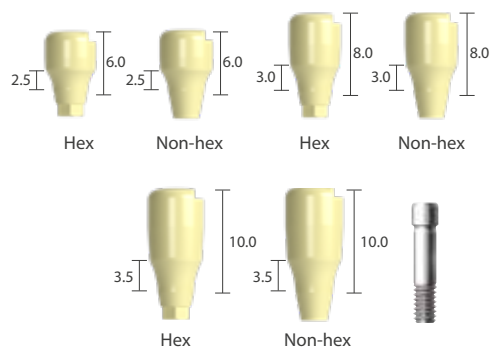

| Diameter | G/H | H | Type | Art. No. |
|----------|-----|------|---------|--------------|
| Ø 6.0 | 2.5 | 6.0 | Hex | IHAB 60 06 H |
| | 2.5 | 6.0 | Non-hex | IHAB 60 06 N |
| | 3.0 | 8.0 | Hex | IHAB 60 08 H |
| | 3.0 | 8.0 | Non-hex | IHAB 60 08 N |
| | 3.5 | 10.0 | Hex | IHAB 60 10 H |
| | 3.5 | 10.0 | Non-hex | IHAB 60 10 N |

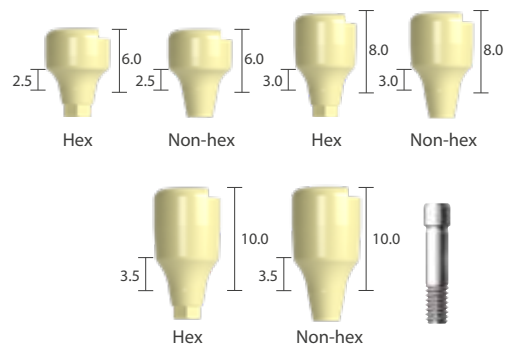

※ Hex driver: Use no more than 10N-cm of torque when screwing Scan Abutment to a fixture.
If hex is worn, slot on the head of the product can be used to rotate it.

Prosthetic Procedure 1

Impression Technique and Restoration Selection

Dual / Combi Abutment

Abutment Level Impression

Closed Tray Technique

Page 14

Combi Abutment

Ø 4.5 / Ø 5.5 / Ø 6.5



Page 15,16

Dual Abutment

Hex / Non-hex
Ø 4.5 / Ø 5.5 / Ø 6.5



Page 17

Impression Coping

Transfer (Snap on)
Ø 4.5 / Ø 5.5 / Ø 6.5



Page 17

Analog

Short
Ø 4.5 / Ø 5.5 / Ø 6.5



Page 17

Analog

Long
Ø 4.5 / Ø 5.5 / Ø 6.5



Burn-out Cylinder

Page 17

Bridge

Rotational
Ø 4.5 / Ø 5.5 / Ø 6.5



Page 17

Single

Non-rotational
Ø 4.5 / Ø 5.5 / Ø 6.5




Modification

Cemented Restoration


Combi Abutment

Unit: mm, Scale 1 : 1

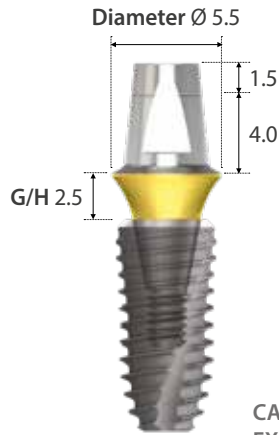


CAB5525
FXS4510


| Diameter | G/H | Type | Art. No. | Type | Art. No. |
|----------|-----|-------|-------------|------|-----------|
| Ø 4.5 | 1.0 | Short | CAB 45 10 S | Long | CAB 45 10 |
| | 1.5 | | CAB 45 15 S | | CAB 45 15 |
| | 2.5 | | CAB 45 25 S | | CAB 45 25 |
| | 3.5 | | CAB 45 35 S | | CAB 45 35 |
| | 4.5 | | CAB 45 45 S | | CAB 45 45 |
| | 5.5 | | CAB 45 55 S | | CAB 45 55 |

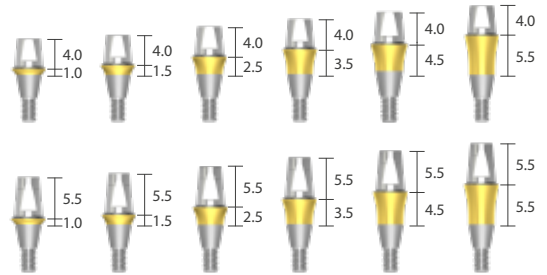

| | | | | | |
|-------|-----|-------|-------------|------|-----------|
| Ø 5.5 | 1.5 | Short | CAB 55 15 S | Long | CAB 55 15 |
| | 2.5 | | CAB 55 25 S | | CAB 55 25 |
| | 3.5 | | CAB 55 35 S | | CAB 55 35 |
| | 4.5 | | CAB 55 45 S | | CAB 55 45 |
| | 5.5 | | CAB 55 55 S | | CAB 55 55 |

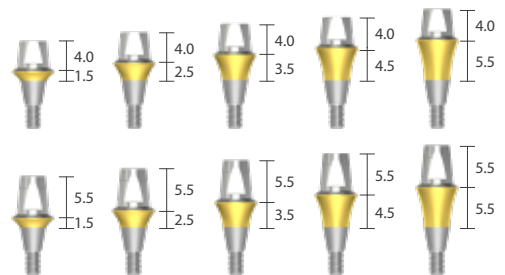

| | | | | | |
|-------|-----|-------|-------------|------|-----------|
| Ø 6.5 | 1.5 | Short | CAB 65 15 S | Long | CAB 65 15 |
| | 2.5 | | CAB 65 25 S | | CAB 65 25 |
| | 3.5 | | CAB 65 35 S | | CAB 65 35 |
| | 4.5 | | CAB 65 45 S | | CAB 65 45 |
| | 5.5 | | CAB 65 55 S | | CAB 65 55 |

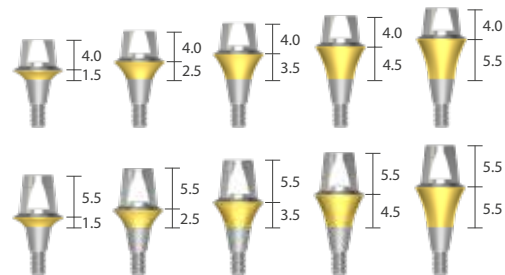


※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Combi Abutment with fixture.




Dual Abutment [Hex]

Unit: mm, Scale 1.5 : 1

· Abutment screw is included

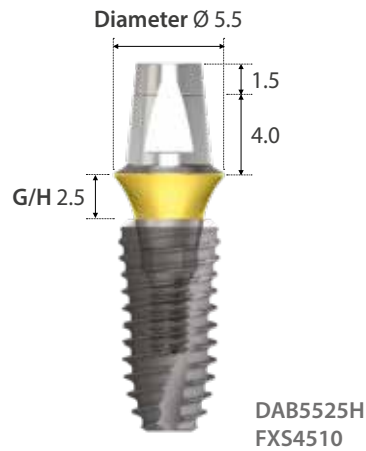

| Diameter | G/H | Art. No. |
|----------|-----|-------------|
| Ø 4.5 | 1.0 | DAB 45 10 H |
| | 1.5 | DAB 45 15 H |
| | 2.5 | DAB 45 25 H |
| | 3.5 | DAB 45 35 H |
| | 4.5 | DAB 45 45 H |
| | 5.5 | DAB 45 55 H |
| Ø 5.5 | 1.5 | DAB 55 15 H |
| | 2.5 | DAB 55 25 H |
| | 3.5 | DAB 55 35 H |
| | 4.5 | DAB 55 45 H |
| | 5.5 | DAB 55 55 H |
| Ø 6.5 | 1.5 | DAB 65 15 H |
| | 2.5 | DAB 65 25 H |
| | 3.5 | DAB 65 35 H |
| | 4.5 | DAB 65 45 H |
| | 5.5 | DAB 65 55 H |

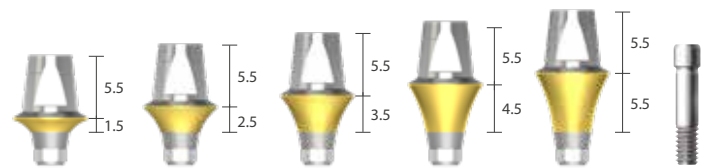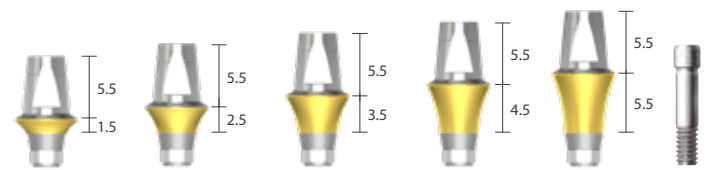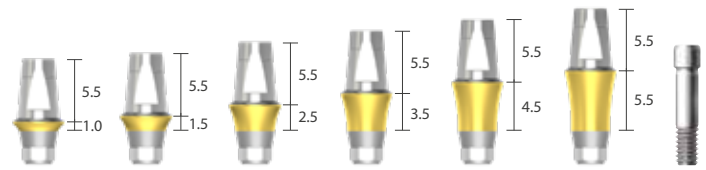


※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Dual Abutment with fixture.


Dual Abutment [Non-hex]

Unit: mm, Scale 1.5 : 1

· Abutment screw is included

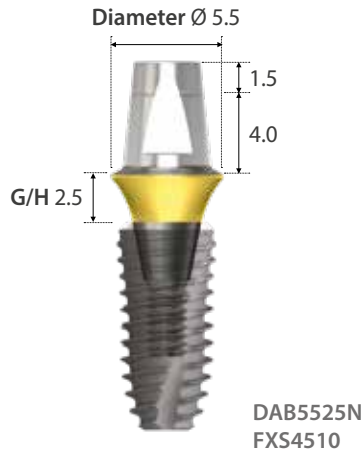

| Diameter | G/H | Art. No. |
|----------|-----|-------------|
| Ø 4.5 | 1.0 | DAB 45 10 N |
| | 1.5 | DAB 45 15 N |
| | 2.5 | DAB 45 25 N |
| | 3.5 | DAB 45 35 N |
| | 4.5 | DAB 45 45 N |
| | 5.5 | DAB 45 55 N |
| Ø 5.5 | 1.5 | DAB 55 15 N |
| | 2.5 | DAB 55 25 N |
| | 3.5 | DAB 55 35 N |
| | 4.5 | DAB 55 45 N |
| | 5.5 | DAB 55 55 N |
| Ø 6.5 | 1.5 | DAB 65 15 N |
| | 2.5 | DAB 65 25 N |
| | 3.5 | DAB 65 35 N |
| | 4.5 | DAB 65 45 N |
| | 5.5 | DAB 65 55 N |

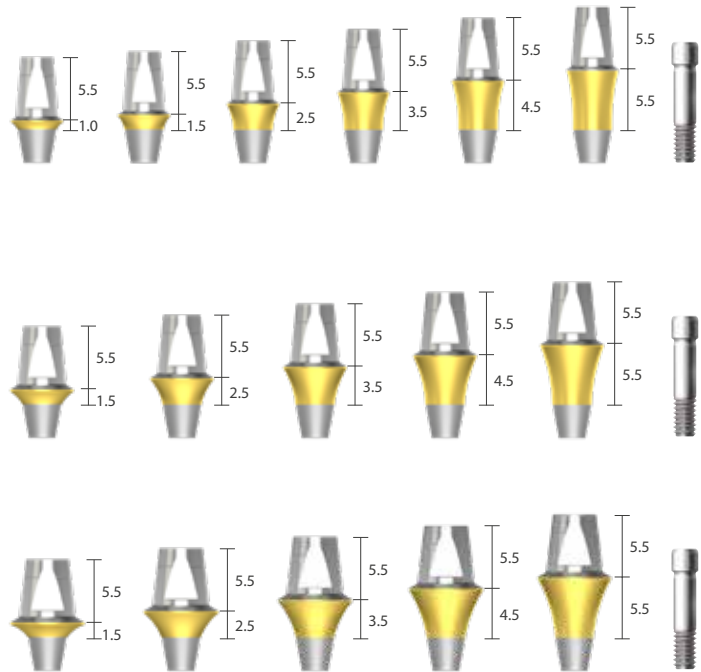


※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Dual Abutment with fixture.

Abutment Level Impression Components

Unit: mm, Scale 1 : 1

Comfort Cap | Snap on

| Type | Diameter | Art. No. |
|-------|----------|-----------|
| Short | Ø 4.5 | CCC 45 CS |
| | Ø 5.5 | CCC 55 CS |
| | Ø 6.5 | CCC 65 CS |
| Long | Ø 4.5 | CCC 45 C |
| | Ø 5.5 | CCC 55 C |
| | Ø 6.5 | CCC 65 C |

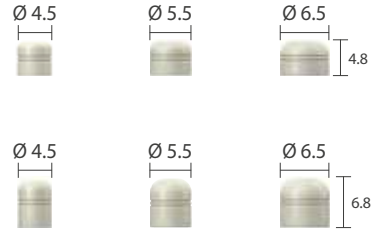


Impression Coping | Snap on

| Diameter | Art. No. |
|----------|----------|
| Ø 4.5 | CIC 45 L |
| Ø 5.5 | CIC 55 L |
| Ø 6.5 | CIC 65 L |



Lab Analog

| Type | Diameter | Art. No. |
|-------|----------|-----------|
| Short | Ø 4.5 | CAN 45 SL |
| | Ø 5.5 | CAN 55 SL |
| | Ø 6.5 | CAN 65 SL |
| Long | Ø 4.5 | CAN 45 LL |
| | Ø 5.5 | CAN 55 LL |
| | Ø 6.5 | CAN 65 LL |

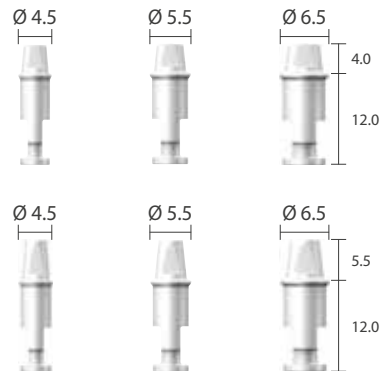

Burn-out Cylinder

| Type | Diameter | Art. No. |
|--------|----------|-----------|
| Single | Ø 4.5 | CBC 45 SL |
| | Ø 5.5 | CBC 55 SL |
| | Ø 6.5 | CBC 65 SL |
| Bridge | Ø 4.5 | CBC 45 BL |
| | Ø 5.5 | CBC 55 BL |
| | Ø 6.5 | CBC 65 BL |



Restorative Kit



Combi & Dual Abutment


| Art. No | Lab. Components | | | | |
|------------------------|-----------------------|-------------------|------------------------|-------------------|-----------|
| | Comfort Cap | Impression Coping | Analog | Burn-out Cylinder | |
| XSDAB 45 S XSDAB 45 | CCC 45 CS CCC 45 C | CIC 45 L | CAN 45 SL CAN 45 LL | CBC 45 SL | CBC 45 BL |
| XSDAB 55 S XSDAB 55 | CCC 55 CS CCC 55 C | CIC 55 L | CAN 55 SL CAN 55 LL | CBC 55 SL | CBC 55 BL |
| XSDAB 65 S XSDAB 65 | CCC 65 CS CCC 65 C | CIC 65 L | CAN 65 SL CAN 65 LL | CBC 65 SL | CBC 65 BL |

Prosthetic Procedure 2

Impression Technique and Restoration Selection

**Dual / Custom / Milling / Angled / Direct-Casting / Metal-Casting /
Ti-Temporary / Plastic Temporary Abutment**

Fixture Level Impression

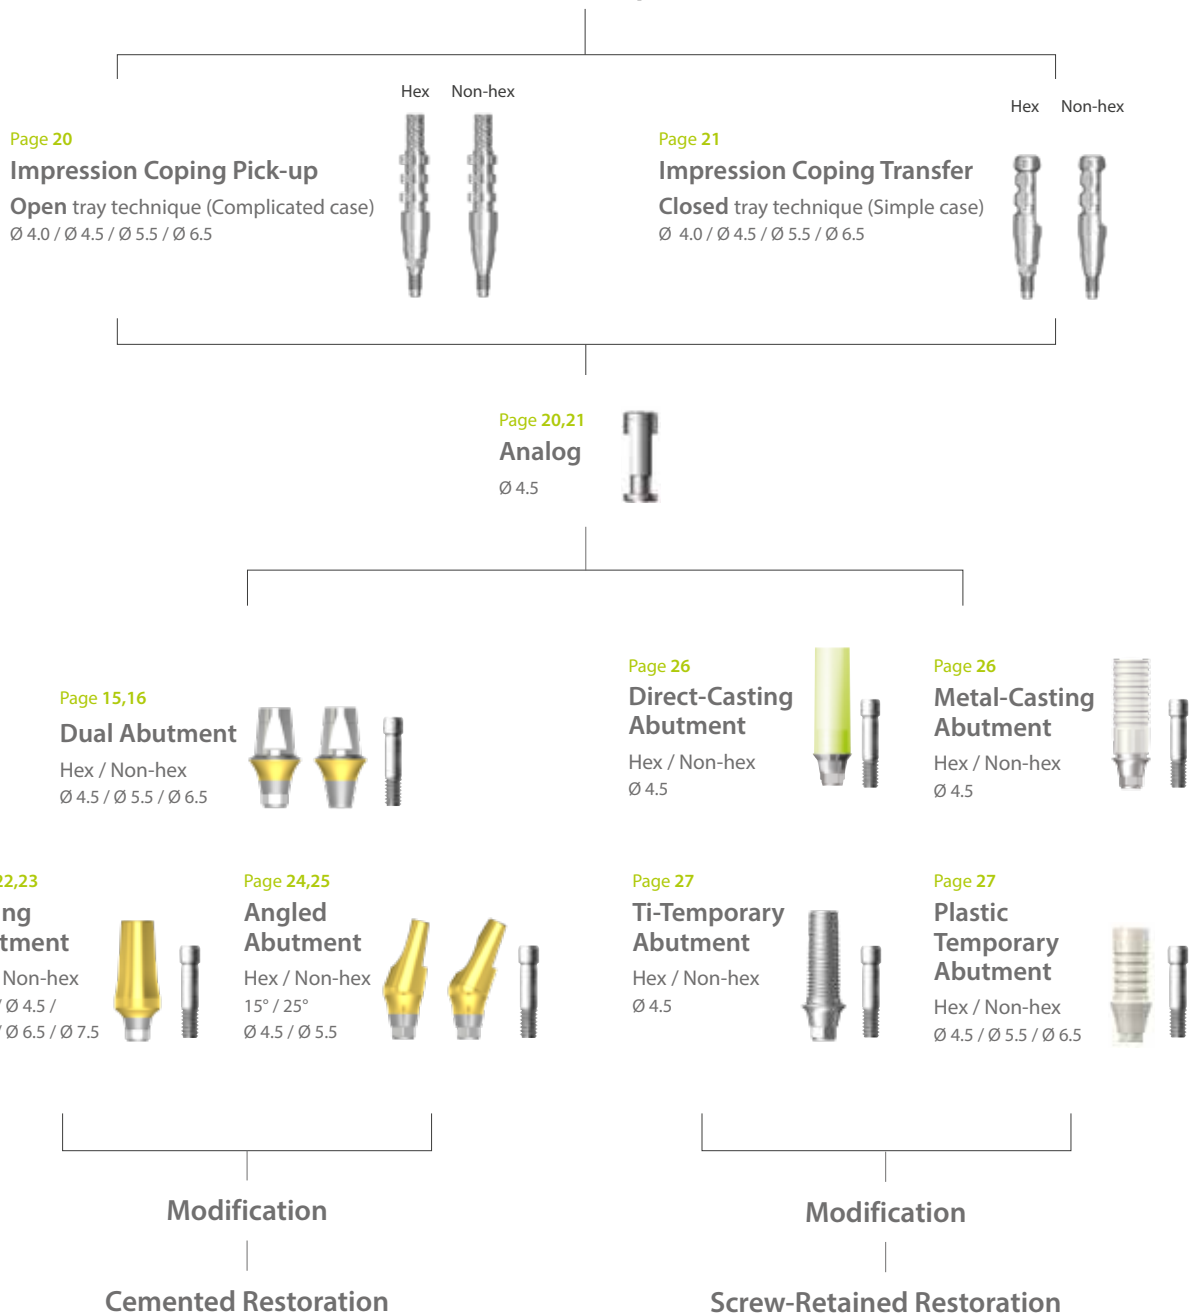


Fixture Level Impression Components

Unit: mm, Scale 1 : 1


· Impression coping screw is included with Impression coping.

Impression Coping Pick-up


| Diameter | Size | Type | Art. No. |
|----------|-------|---------|--------------|
| Ø 4.0 | Short | Hex | DPU 40 11 HE |
| | Short | Non-hex | DPU 40 11 NE |
| | Long | Hex | DPU 40 15 HE |
| | Long | Non-hex | DPU 40 15 NE |

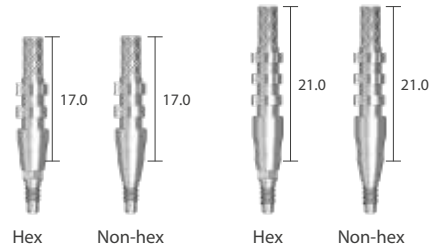


| | | | |
|-------|-------|---------|--------------|
| Ø 4.5 | Short | Hex | DPU 45 11 HE |
| | Short | Non-hex | DPU 45 11 NE |
| | Long | Hex | DPU 45 15 HE |
| | Long | Non-hex | DPU 45 15 NE |

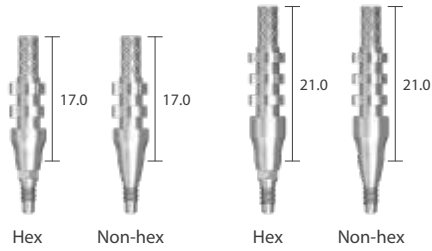

| | | | |
|-------|-------|---------|--------------|
| Ø 5.5 | Short | Hex | DPU 55 11 HE |
| | Short | Non-hex | DPU 55 11 NE |
| | Long | Hex | DPU 55 15 HE |
| | Long | Non-hex | DPU 55 15 NE |

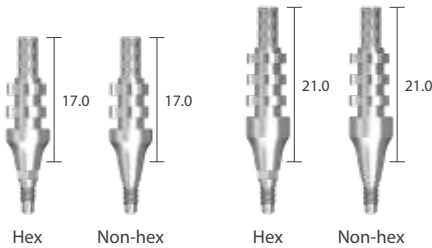


| | | | |
|-------|-------|---------|--------------|
| Ø 6.5 | Short | Hex | DPU 65 11 HE |
| | Short | Non-hex | DPU 65 11 NE |
| | Long | Hex | DPU 65 15 HE |
| | Long | Non-hex | DPU 65 15 NE |

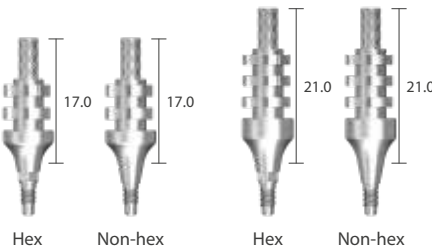


Impression Coping Transfer Screw

| Size | L | Art. No. |
|-------|------|----------|
| Short | 23.0 | DPS 11 E |
| Long | 27.0 | DPS 15 E |



Analog

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 4.5 | 12.0 | DANSE |




Fixture Level Impression Components

Unit: mm, Scale 1 : 1


· Impression coping screw is included with Impression coping.

Impression Coping Transfer


| Diameter | Size | Type | Art. No. |
|----------|-------|---------|--------------|
| Ø 4.0 | Short | Hex | DTF 40 11 HE |
| | Short | Non-hex | DTF 40 11 NE |
| | Long | Hex | DTF 40 15 HE |
| | Long | Non-hex | DTF 40 15 NE |

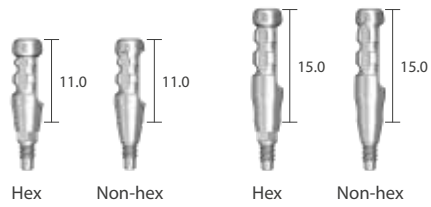


| | | | |
|-------|-------|---------|--------------|
| Ø 4.5 | Short | Hex | DTF 45 11 HE |
| | Short | Non-hex | DTF 45 11 NE |
| | Long | Hex | DTF 45 15 HE |
| | Long | Non-hex | DTF 45 15 NE |

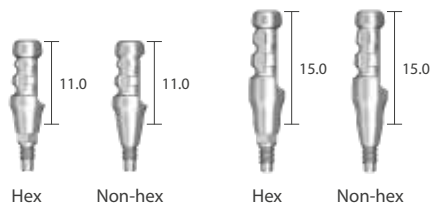

| | | | |
|-------|-------|---------|--------------|
| Ø 5.5 | Short | Hex | DTF 55 11 HE |
| | Short | Non-hex | DTF 55 11 NE |
| | Long | Hex | DTF 55 15 HE |
| | Long | Non-hex | DTF 55 15 NE |

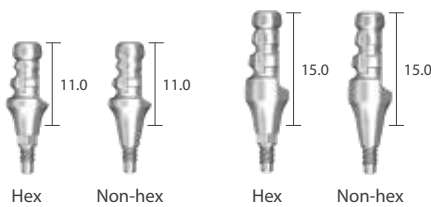


| | | | |
|-------|-------|---------|--------------|
| Ø 6.5 | Short | Hex | DTF 65 11 HE |
| | Short | Non-hex | DTF 65 11 NE |
| | Long | Hex | DTF 65 15 HE |
| | Long | Non-hex | DTF 65 15 NE |

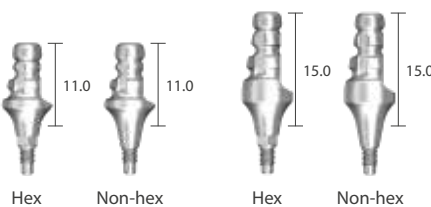


Impression Coping Transfer Screw

| Size | L | Art. No. |
|-------|------|----------|
| Short | 17.0 | DTS 11 E |
| Long | 21.0 | DTS 15 E |



Analog

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 4.5 | 12.0 | DANSE |




Milling Abutment

Unit: mm, Scale 1.5 : 1


· Abutment screw is included.




| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|--------------|
| Ø 4.0 | 1.0 | Hex | MAB 40 105 H |
| | 1.0 | Non-hex | MAB 40 105 N |



| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|--------------|
| Ø 4.5 | 1.5 | Hex | MAB 45 156 H |
| | 1.5 | Non-hex | MAB 45 156 N |



| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|--------------|
| Ø 5.5 | 1.5 | Hex | MAB 55 157 H |
| | 1.5 | Non-hex | MAB 55 157 N |
| | 2.5 | Hex | MAB 55 257 H |
| | 2.5 | Non-hex | MAB 55 257 N |

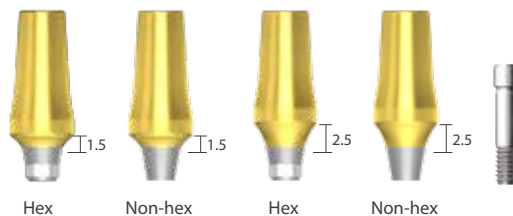


※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Milling Abutment with fixture.

Milling Abutment

Unit: mm, Scale 1.5 : 1

· Abutment screw is included.

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|--------------|
| Ø 6.5 | 1.5 | Hex | MAB 65 158 H |
| | 1.5 | Non-hex | MAB 65 158 N |
| | 2.5 | Hex | MAB 65 258 H |
| | 2.5 | Non-hex | MAB 65 258 N |
| | 3.5 | Hex | MAB 65 358 H |
| | 3.5 | Non-hex | MAB 65 358 N |

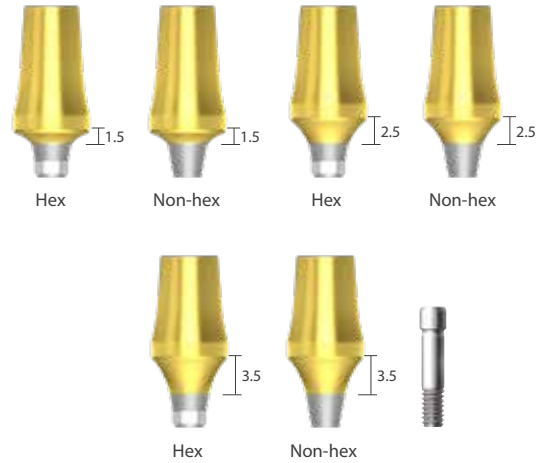

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|--------------|
| Ø 7.5 | 2.5 | Hex | MAB 75 259 H |
| | 2.5 | Non-hex | MAB 75 259 N |
| | 3.5 | Hex | MAB 75 359 H |
| | 3.5 | Non-hex | MAB 75 359 N |




※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Milling Abutment with fixture.


Angled Abutment [15°]

Unit: mm, Scale 1.5 : 1


· Abutment screw is included.

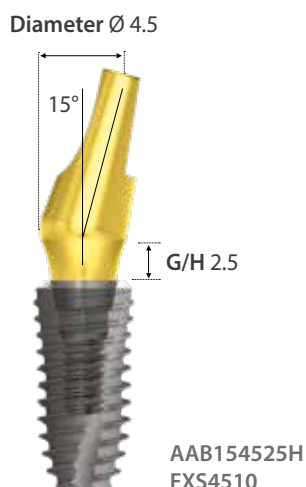

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|----------------|
| Ø 4.5 | 1.5 | Hex | AAB 15 45 15 H |
| | 1.5 | Non-hex | AAB 15 45 15 N |
| | 2.5 | Hex | AAB 15 45 25 H |
| | 2.5 | Non-hex | AAB 15 45 25 N |
| | 3.5 | Hex | AAB 15 45 35 H |
| | 3.5 | Non-hex | AAB 15 45 35 N |

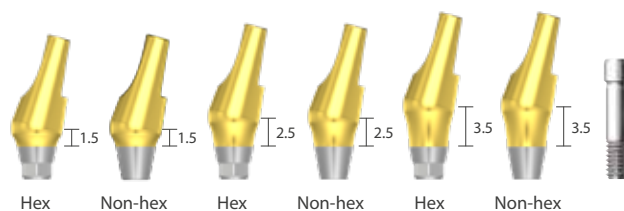

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|----------------|
| Ø 5.5 | 1.5 | Hex | AAB 15 55 15 H |
| | 1.5 | Non-hex | AAB 15 55 15 N |
| | 2.5 | Hex | AAB 15 55 25 H |
| | 2.5 | Non-hex | AAB 15 55 25 N |
| | 3.5 | Hex | AAB 15 55 35 H |
| | 3.5 | Non-hex | AAB 15 55 35 N |

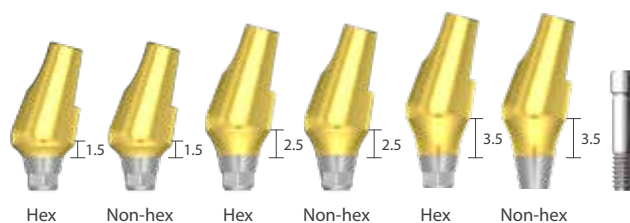


※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Angled Abutment with fixture.

Angled Abutment [25°]

Unit: mm, Scale 1.5 : 1

· Abutment screw is included.

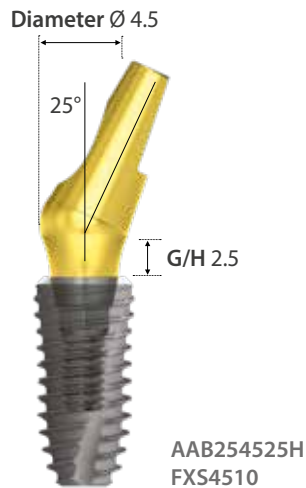

| Diameter | G/H | Type | Art. No. |
|-------------------|-----|---------|----------------|
| \varnothing 4.5 | 1.5 | Hex | AAB 25 45 15 H |
| | 1.5 | Non-hex | AAB 25 45 15 N |
| | 2.5 | Hex | AAB 25 45 25 H |
| | 2.5 | Non-hex | AAB 25 45 25 N |
| | 3.5 | Hex | AAB 25 45 35 H |
| | 3.5 | Non-hex | AAB 25 45 35 N |



| Diameter | G/H | Type | Art. No. |
|-------------------|-----|---------|----------------|
| \varnothing 5.5 | 1.5 | Hex | AAB 25 55 15 H |
| | 1.5 | Non-hex | AAB 25 55 15 N |
| | 2.5 | Hex | AAB 25 55 25 H |
| | 2.5 | Non-hex | AAB 25 55 25 N |
| | 3.5 | Hex | AAB 25 55 35 H |
| | 3.5 | Non-hex | AAB 25 55 35 N |




※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Angled Abutment with fixture.

Direct-Casting Abutment


Unit: mm, Scale 1.5 : 1

• Abutment screw is included.

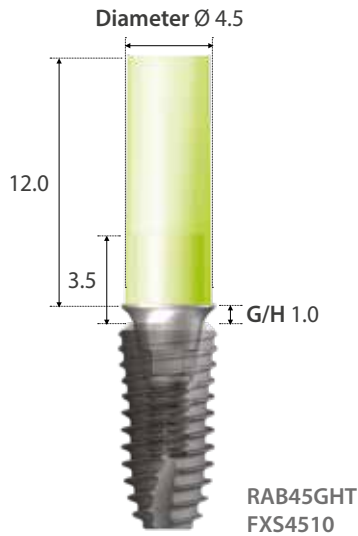

Gold

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|------------|
| Ø 4.5 | 1.0 | Hex | RAB 45 GHT |
| | | Non-hex | RAB 45 GNT |



Metal-Casting Abutment


Unit: mm, Scale 1.5 : 1

• Abutment screw is included.



Co-Cr

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|------------|
| Ø 4.5 | 1.0 | Hex | RAB 45 CLH |
| | | Non-hex | RAB 45 CLN |




※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Direct/Metal Casting Abutment with fixture.

Ti-Temporary Abutment

• Abutment screw is included.

Unit: mm, Scale 1.5 : 1

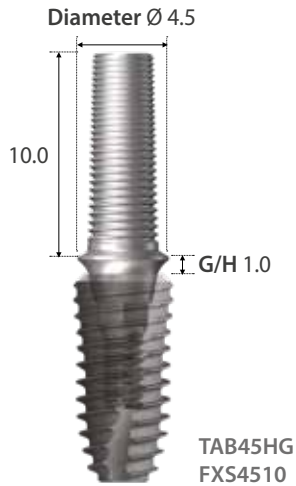

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|-------------|
| Ø 4.5 | 1.0 | Hex | TAB 4510 HG |
| | | Non-hex | TAB 4510 NG |
| | 3.0 | Hex | TAB 4530 HG |
| | | Non-hex | TAB 4530 NG |




Plastic Temporary Abutment

• Abutment screw is included.

Unit: mm, Scale 1.5 : 1



| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|---------------|
| Ø 4.5 | 2.0 | Hex | RAB 45 20 PHL |
| | | Non-hex | RAB 45 20 PNL |
| Ø 5.5 | 2.0 | Hex | RAB 55 20 PHL |
| | | Non-hex | RAB 55 20 PNL |
| Ø 6.5 | 2.0 | Hex | RAB 65 20 PHL |
| | | Non-hex | RAB 65 20 PNL |

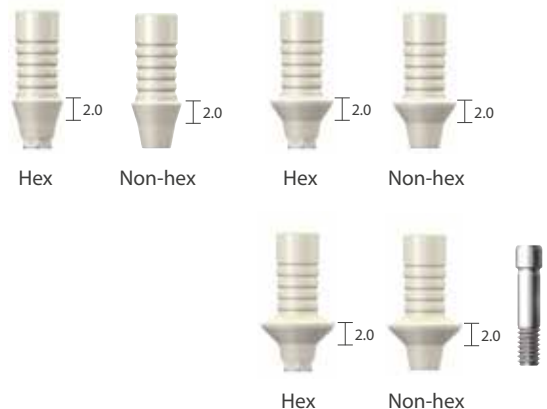


※ Hex driver: It is recommended to keep the torque level at 15~20 N-cm to tighten Temporary Abutment with fixture.

Prosthetic Procedure 3

Impression Technique and Restoration Selection


Screw Abutment

Abutment Level Impression

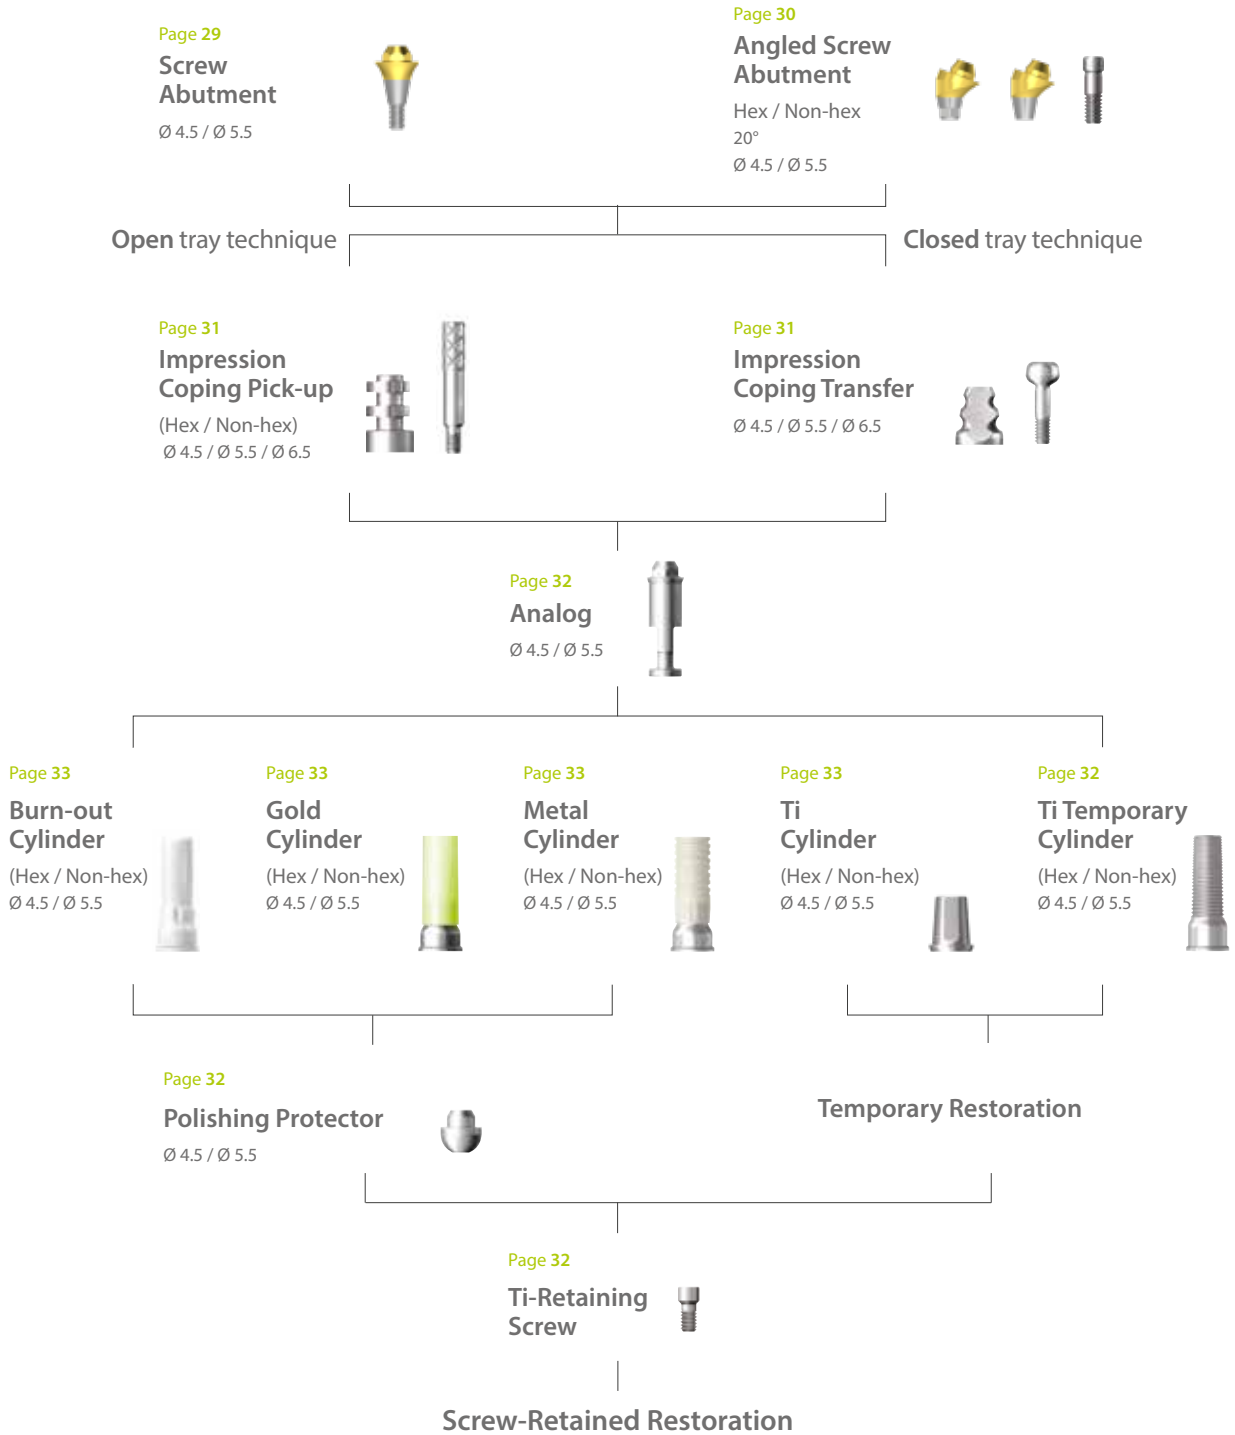


Screw Abutment


Unit: mm, Scale 1.5 : 1

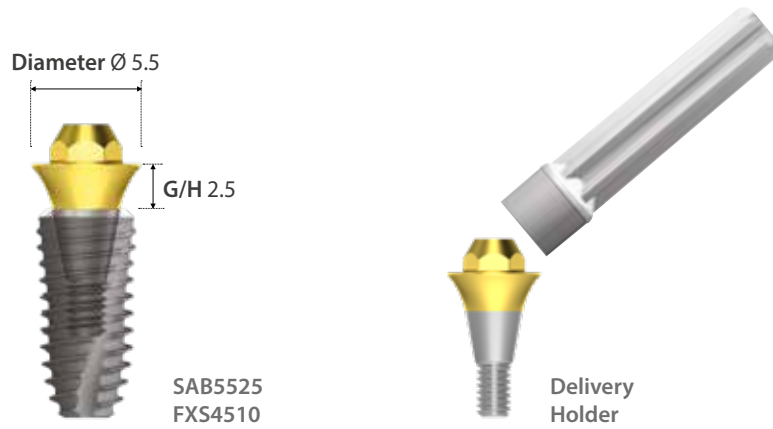

| Diameter | G/H | Art. No. |
|-------------------|-----|-----------|
| \varnothing 4.5 | 1.0 | SAB 45 10 |
| | 1.5 | SAB 45 15 |
| | 2.5 | SAB 45 25 |
| | 3.5 | SAB 45 35 |
| | 4.5 | SAB 45 45 |
| | 5.5 | SAB 45 55 |

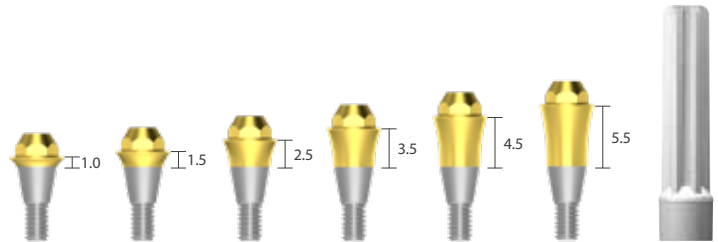

| Diameter | G/H | Art. No. |
|-------------------|-----|-----------|
| \varnothing 5.5 | 1.5 | SAB 55 15 |
| | 2.5 | SAB 55 25 |
| | 3.5 | SAB 55 35 |
| | 4.5 | SAB 55 45 |
| | 5.5 | SAB 55 55 |

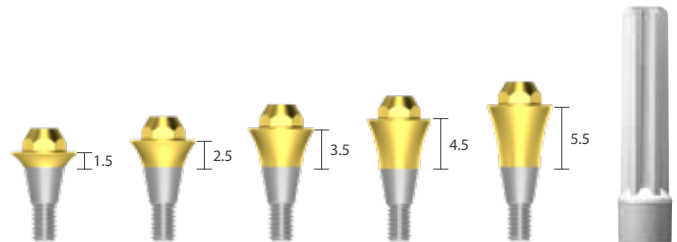


※ Hex driver: It is recommended to keep the torque level at 30~35 N-cm to tighten Screw Abutment with fixture.


Angled Screw Abutment

Unit: mm, Scale 1.5 : 1


· Abutment screw is included.

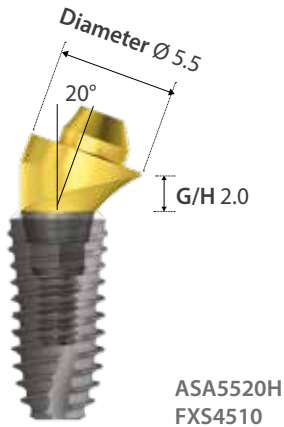

| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|-------------|
| Ø 4.5 | 1.0 | Hex | ASA 45 10 H |
| | 1.0 | Non-hex | ASA 45 10 N |
| | 2.0 | Hex | ASA 45 20 H |
| | 2.0 | Non-hex | ASA 45 20 N |
| | 3.0 | Hex | ASA 45 30 H |
| | 3.0 | Non-hex | ASA 45 30 N |

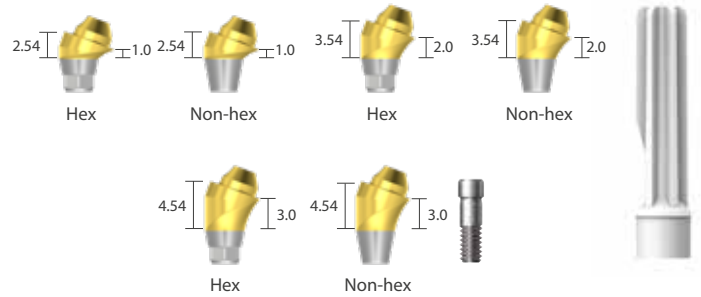


| Diameter | G/H | Type | Art. No. |
|----------|-----|---------|-------------|
| Ø 5.5 | 1.0 | Hex | ASA 55 10 H |
| | 1.0 | Non-hex | ASA 55 10 N |
| | 2.0 | Hex | ASA 55 20 H |
| | 2.0 | Non-hex | ASA 55 20 N |
| | 3.0 | Hex | ASA 55 30 H |
| | 3.0 | Non-hex | ASA 55 30 N |

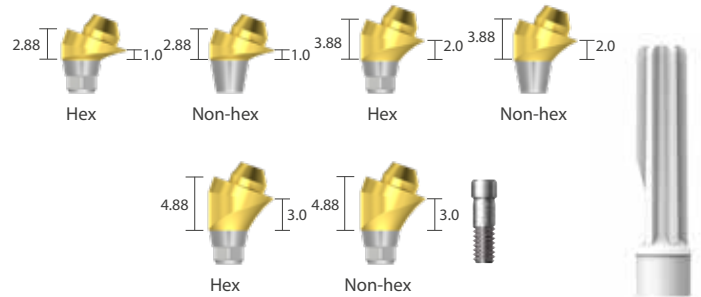

Angled Screw Abutment Screw

| Diameter | L | Art. No. |
|----------|-----|-------------|
| Ø 2.3 | 7.3 | ASASC 20 23 |



Ti-Delivery Holder

| |
|------|
| ASAH |
|------|



※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Angled Screw Abutment with fixture.

Screw Abutment Impression Components

Unit: mm, Scale 1.5 : 1

Impression Coping Pick-up

| Diameter | Type | Art. No. |
|----------|---------|-----------|
| Ø 4.5 | Hex | SPU 45 SL |
| | Non-hex | SPU 45 BL |
| Ø 5.5 | Hex | SPU 55 SL |
| | Non-hex | SPU 55 BL |

Ø 4.5



Hex

Ø 4.5



Non-hex

Ø 5.5



Hex

Ø 5.5



Non-hex

Impression Coping Transfer

| Diameter | Type | Art. No. |
|----------|---------|-----------|
| Ø 4.5 | Hex | STF 45 SL |
| | Non-hex | STF 45 BL |
| Ø 5.5 | Hex | STF 55 SL |
| | Non-hex | STF 55 BL |

Ø 4.5



Hex

Ø 4.5



Non-hex

Ø 5.5



Hex

Ø 5.5



Non-hex

Impression Coping Screw

| Type | L | Art. No. |
|----------|------|----------|
| Pick-up | 15.0 | SPS 09 |
| Transfer | 9.0 | STS 09 |



15.0



9.0

Screw Abutment Components

Unit: mm, Scale 1.5 : 1


Comfort Cap

| Diameter | L | Art. No. |
|----------|-----|----------|
| Ø 4.5 | 5.0 | SCC 45 L |
| Ø 5.5 | | SCC 55 L |




Scan Comfort Cap | PEEK

| Diameter | L | Art. No. | |
|----------|-----|----------|-----------|
| Ø 4.5 | 5.0 | Hex | ISC 45 SP |
| | | Non-hex | ISC 45 BP |
| Ø 5.5 | | Hex | ISC 55 SP |
| | | Non-hex | ISC 55 BP |



Analog

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 4.5 | 12.0 | SAN 45 L |
| Ø 5.5 | | SAN 55 L |




Polishing Protector

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 4.5 | 4.71 | SPP 45 L |
| Ø 5.5 | | SPP 55 L |




Ti-Retaining Screw

| Diameter | L | Art. No. |
|----------|-----|----------|
| Ø 2.3 | 5.0 | SRS 18 T |



Ti-Temporary Cylinder

| Diameter | Type | Art. No. |
|----------|---------|-----------|
| Ø 4.5 | Hex | STC 45 SG |
| | Non-hex | STC 45 BG |
| Ø 5.5 | Hex | STC 55 SG |
| | Non-hex | STC 55 BG |




Screw Abutment Components

Unit: mm, Scale 1.5 : 1

Ti-Cylinder

| Diameter | Type | Art. No. |
|----------|---------|----------|
| Ø 4.5 | Hex | STA 45 S |
| | Non-hex | STA 45 B |
| Ø 5.5 | Hex | STA 55 S |
| | Non-hex | STA 55 B |

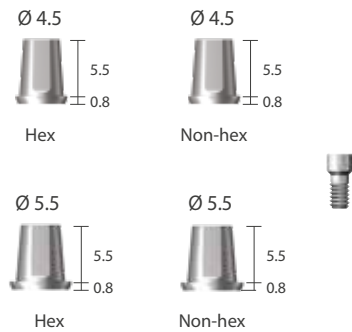

Gold Cylinder

| Diameter | Type | Art. No. |
|----------|---------|-----------|
| Ø 4.5 | Hex | SGC 45 SL |
| | Non-hex | SGC 45 BL |
| Ø 5.5 | Hex | SGC 55 SL |
| | Non-hex | SGC 55 BL |



Metal Cylinder | Co-Cr

| Diameter | Type | Art. No. |
|----------|---------|------------|
| Ø 4.5 | Hex | SGC 45 CSL |
| | Non-hex | SGC 45 CBL |
| Ø 5.5 | Hex | SGC 55 CSL |
| | Non-hex | SGC 55 CBL |



Burn-out Cylinder

| Diameter | Type | Art. No. |
|----------|---------|-----------|
| Ø 4.5 | Hex | SBC 45 SL |
| | Non-hex | SBC 45 BL |
| Ø 5.5 | Hex | SBC 55 SL |
| | Non-hex | SBC 55 BL |



※ Hex driver: It is recommended to keep the torque level at 15~20 N-cm to tighten Screw Abutment Components with fixture.

Prosthetic Procedure 4

Impression Technique and Restoration Type

Overdenture Procedure

Positioner / Mini Ball / Magnetic Attachment

Page 35

Positioner Abutment

Ø 3.5



Page 37

Mini Ball Abutment

Ø 3.3 / Ø 3.5



Page 38,39

Magnetic Implant Keeper

Dome type / Flat type
Ø 4.5 / Ø 5.5



Abutment Level Impression

Page 35

Positioner Impression Coping

Ø 4.5



Page 37

Mini Ball Impression Coping

Ø 3.5



Page 35

Positioner Analog

Ø 3.5



Page 37

Mini Ball Analog

Ø 3.5



Page 37

Socket Spacer


Ø 4.05 / Ø 4.85



Page 36

Positioner Socket

Metal / Plastic



Page 37

Mini Ball Female Socket / O-ring

Ø 4.05 / Ø 4.85



Page 38,39

Magnetic Assay

Dome type / Flat type
Ø 4.5 / Ø 5.5




Positioner Attachment for Overdenture

Mini Ball and Socket Attachment for Overdenture

Magnetic Attachment for Overdenture


Positioner

Unit: mm, Scale 1.5 : 1

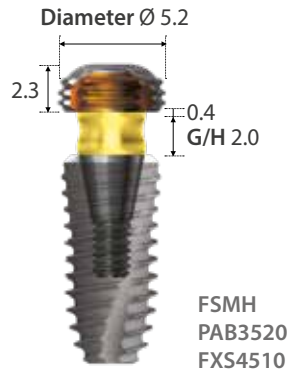

Positioner Abutment

| Diameter | G/H | Art. No. |
|----------|-----|-----------|
| Ø 3.5 | 1.0 | PAB 35 10 |
| | 2.0 | PAB 35 20 |
| | 3.0 | PAB 35 30 |
| | 4.0 | PAB 35 40 |
| | 5.0 | PAB 35 50 |
| | 6.0 | PAB 35 60 |
| | 7.0 | PAB 35 70 |

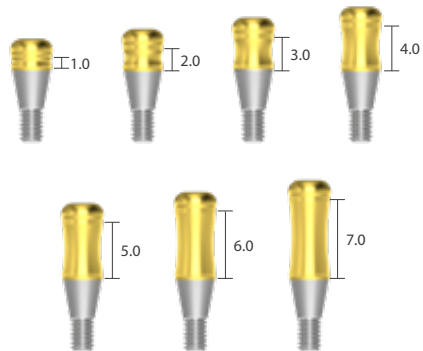


Positioner Impression Coping

| Diameter | L | Art. No. |
|----------|-----|----------|
| Ø 4.5 | 4.5 | PIC |



Positioner Analog

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 3.5 | 12.4 | PAN |



※ Hex driver: It is recommended to keep the torque level at 30~35 N-cm to tighten Positioner Abutment with fixture.

Positioner

Unit: mm, Scale 1.5 : 1


Positioner Socket Set

| Type | Art. No. |
|--------------------------------|----------|
| Tilting type $\pm 10^\circ$ | FSMHS |
| Non Tilting type $\pm 5^\circ$ | FSMHSN |




Positioner Metal Socket

| Diameter | H | Art. No. |
|-------------------|-----|----------|
| $\varnothing 5.2$ | 2.3 | FSMH |



Plastic Scket

| Type | Application | Art. No. |
|--------------------------------|--------------|----------|
| Tilting type $\pm 10^\circ$ | Blue 1,000gf | MSHP |
| | Orange 500gf | MSMP |
| | Ivory 300gf | MSLP |
| | White 100gf | MSOP |
| Non tilting type $\pm 5^\circ$ | Blue 1000gf | MSHPN |
| | Orange 500gf | MSMPN |
| | Ivory 300gf | MSLPN |
| | White 100gf | MSOPN |

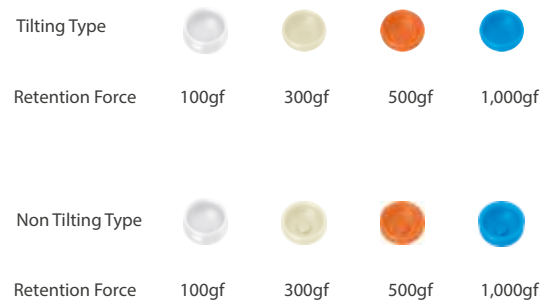

Block Out Spacer

| Diameter | H | Art. No. |
|-------------------|-----|----------|
| $\varnothing 6.5$ | 0.5 | BOS |



Positioner Core Tool

| |
|------|
| XPCT |
|------|




Mini Ball Attachment

Unit: mm, Scale 1.5 : 1




Mini Ball Abutment

| Diameter | G/H | Art. No. |
|----------|-----|--------------|
| Ø 3.3 | 0 | BAB 35 00 18 |
| Ø 3.5 | 1.0 | BAB 35 10 18 |
| Ø 3.5 | 2.0 | BAB 35 20 18 |
| Ø 3.5 | 3.0 | BAB 35 30 18 |
| Ø 3.5 | 4.0 | BAB 35 40 18 |
| Ø 3.5 | 5.0 | BAB 35 50 18 |

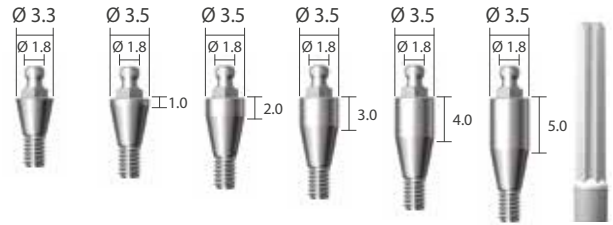

Mini Ball Impression Coping

| Diameter | L | Art. No. |
|----------|-----|----------|
| Ø 3.4 | 4.2 | GICA |



Mini Ball Analog

| Diameter | Art. No. |
|----------|----------|
| Ø 3.5 | BANL |




Socket Spacer

| Diameter | Art. No. |
|----------|----------|
| Ø 4.05 | GBIC 3 L |
| Ø 4.85 | GBIC 2 L |



Female Socket

| Diameter | Retention Force | Art. No. |
|----------|-----------------|----------|
| Ø 4.05 | 300~500gf | BPF 3 |
| Ø 4.85 | 500~700gf | BPF 2 |



Block Out Spacer


| Diameter | H | Art. No. |
|----------|-----|----------|
| Ø 6.5 | 0.5 | BOS |



※ Hex driver: It is recommended to keep the torque level at 30~35 N-cm to tighten Mini Ball Abutment with fixture.

Magnetic Attachment [Dome Type]


Unit: mm, Scale 1.5 : 1

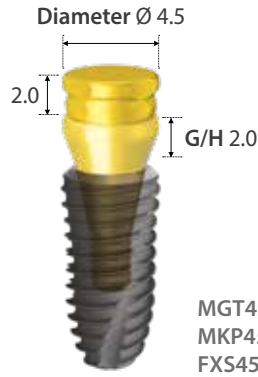

MGT4520D
MKP4520D
FXS4510


Magnetic Assay

| Application | Diameter | H | Art. No. |
|-------------|----------|-----|-------------|
| MKP45D | Ø 4.5 | 2.0 | MGT 45 20 D |
| MKP55D | Ø 5.5 | 2.0 | MGT 55 20 D |



Implant Keeper Diameter


| Diameter | G/H | Art. No. |
|----------|-----|-------------|
| Ø 4.5 | 1.0 | MKP 45 10 D |
| | 2.0 | MKP 45 20 D |
| | 3.0 | MKP 45 30 D |
| | 4.0 | MKP 45 40 D |
| | 5.0 | MKP 45 50 D |
| | 6.0 | MKP 45 60 D |
| Ø 5.5 | 1.0 | MKP 55 10 D |
| | 2.0 | MKP 55 20 D |
| | 3.0 | MKP 55 30 D |
| | 4.0 | MKP 55 40 D |
| | 5.0 | MKP 55 50 D |
| | 6.0 | MKP 55 60 D |

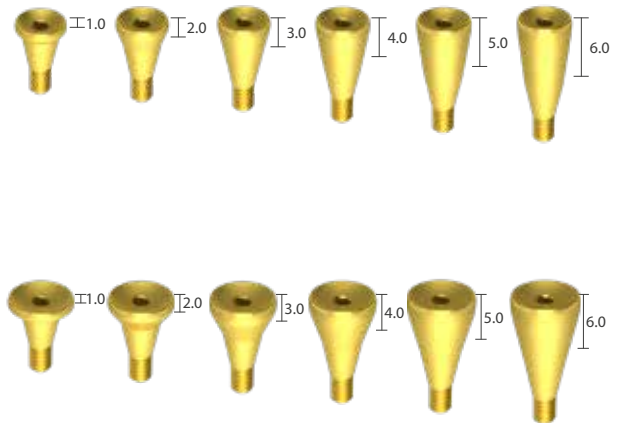

※ Hex driver: It is recommended to keep the torque level at 30~35 N·cm to tighten Magnetic Abutment with fixture.

Magnetic Attachment [Flat Type]

Unit: mm, Scale 1.5 : 1

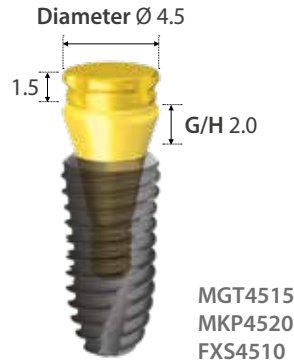


Magnetic Assay

| Application | Diameter | H | Art. No. |
|-------------|----------|-----|-----------|
| MKP 45 | Ø 4.5 | 1.5 | MGT 45 15 |
| | Ø 4.5 | 2.0 | MGT 45 20 |
| MKP 55 | Ø 5.5 | 1.5 | MGT 55 15 |
| | Ø 5.5 | 2.0 | MGT 55 20 |



Implant Keeper Diameter

| Diameter | G/H | Art. No. |
|----------|-----|-----------|
| Ø 4.5 | 1.0 | MKP 45 10 |
| | 2.0 | MKP 45 20 |
| | 3.0 | MKP 45 30 |
| | 4.0 | MKP 45 40 |
| | 5.0 | MKP 45 50 |
| | 6.0 | MKP 45 60 |
| Ø 5.5 | 1.0 | MKP 55 10 |
| | 2.0 | MKP 55 20 |
| | 3.0 | MKP 55 30 |
| | 4.0 | MKP 55 40 |
| | 5.0 | MKP 55 50 |
| | 6.0 | MKP 55 60 |

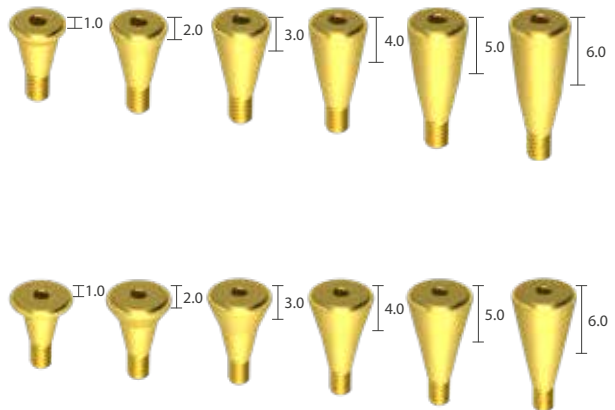


Block Out Spacer

| Diameter | H | Art. No. |
|----------|-----|----------|
| Ø 6.5 | 0.5 | BOS |



※ Hex driver: It is recommended to keep the torque level at 30~35 N-cm to tighten Implant Keeper with fixture.

Surgical Kit [Full]

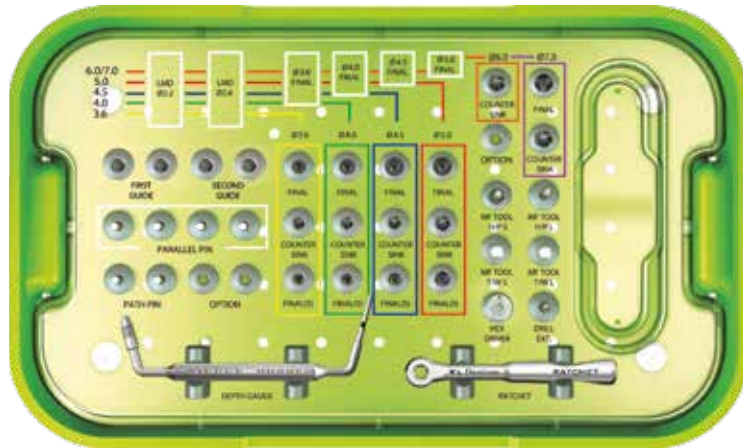

SuperLine Surgical Full Kit

UXNF

Kit Includes

First Guide Drill



XLD2229 XLD2235 (Stopper) XLD2629 XLD2635 (Stopper)

Second Guide Drill



XFD3435 XFD3835

Final Drill



XFD4335 XFD4835

Hand-piece Adapter



XFD5831 XFA27H XFA32H

Parallel Pin



XPP162220T

Countersink



XCS3629SW XCS4029SW XCS4529SW XCS5029SW XCS6029SW XCS7029SW

Ratchet Adapter



XFA26W XFA32W

MF Path Pin



XMFFA2

Final Drill(s)



XFD3429 XFD3829 XFD4329 XFD4829

Hex Driver Drill Extension



XHD26T XDE

Depth Gauge



XDGL

Ratchet



XRCA1

Surgical Kit [Stopper Drill Full]



Stopper Drill Full Kit

UXSF

Kit Includes

First Guide Drill



XLD2208S

Second Guide Drill



XLD2608S

Final Drill



XFD3408S



XFD3808S



XFD4308S



XFD4808S

Hand-piece Adapter



XFD5831



XFA27H



XFA32H



XLD2210S



XLD2610S



XFD3410S



XFD3810S



XFD4310S



XFD4810S

Ratchet Adapter



XFA26W



XFA32W



XLD2212S



XLD2612S



XFD3412S



XFC3812S



XFD4312S



XFD4812S

HexDriver Drill Extension



XHD26T



XDE



XPP162220T

Countersink



XFC3607



XFC4007



XFC4507



XFC5007



XFC6007



XFC7007

Hand-piece Ratchet



XHD25H



XHD25W

MF Path Pin



XMFPA2

Depth Gauge



XDGL

Torque Wrench



XNTW

Surgical Kit [Standard]



SuperLine Surgical Standard Kit

UXNS

Kit Includes

First Guide Drill



XLD2231



XFD3431



XFD3831



XFD4331



XFD4831



XFD5831

Final Drill

Second Guide Drill



XLD2631



XCS3629SW



XCS4029SW



XCS4529SW



XCS5029SW



XCS7029SW

Countersink

Ratchet



XRCA1

Parallel Pin



XPP162220T



XMFPA2

MF Path Pin



XMFPA2

Hex Driver (Hand-piece)



XHD25H



XCS6029SW

Hand-piece Adapter



XFA30H

Hex Driver

Drill Extension

Ratchet Adapter



XPP162226T



XMFPA2



XMFPA2



XHD26T




XDE



XFA26W

Surgical Kit [Short Implant]

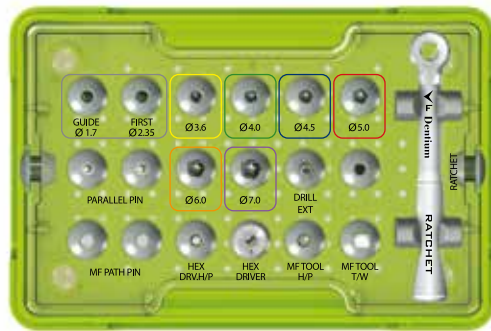

SuperLine Short Implant Surgical Kit

XSIIK

Kit Includes

First Guide Drill



XLD2207

Second Guide Drill



XLD2607

Final Drill



XFC3607



XFC4007



XFC4507



XFC5007

Parallel Pin



XPP162212



XFC6007



XFC7007

Ratchet



MF Path Pin



XMFP A2



Hex Driver



XHD25H



XHD26T

Hand-piece Adapter



XFA27H

Ratchet Adapter



XFA26W

XRCA1



















Surgical Kit [Stopper Drill Kit]




Stopper Drill Kit

XSDK

Kit Includes

| | First Guide Drill | Second Guide Drill | Final Drill | | | |
|-----|---|---|---|---|---|---|
| L8 |  XLD2208S |  XLD2608S |  XFD3408S |  XFD3808S |  XFD4308S |  XFD4808S |
| L10 |  XLD2210S |  XLD2610S |  XFD3410S |  XFD3810S |  XFD4310S |  XFD4810S |
| L12 |  XLD2212S |  XLD2612S |  XFD3412S |  XFD3812S |  XFD4312S |  XFD4812S |

Surgical Kit [Drill Stopper Kit]

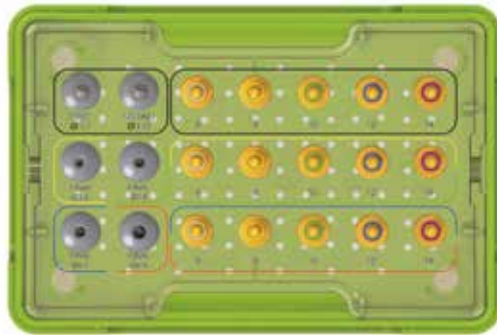

Drill Stopper Kit

XDS

Kit Includes

Guide Drill Stopper
First Second

XLD2235 XLD2635

Stopper - First Guide Drill, Second Guide Drill

XLDST06 XLDST08 XLDST10 XLDST12 XLDST14

Final Drill Stopper
34 38

XFD3435 XFD3835

Stopper - Final Drill / 34, 38

XFDST06 XFDST08 XFDST10 XFDST12 XFDST14

Final Drill Stopper
43 48

XFD4335 XFD4835

Stopper - Final Drill / 43, 48



XFDST06L XFDST08L XFDST10L XFDST12L XFDST14L

Surgical Instruments

Unit: mm, Scale 1 : 1



First Guide Drill

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.2 | 26 | XLD 22 07 |
| | 29 | XLD 22 29 |
| | 31 | XLD 22 31 |
| | 33 | XLD 22 33 |
| | 35 | XLD 22 35 |
| | 41 | XLD 22 41 |

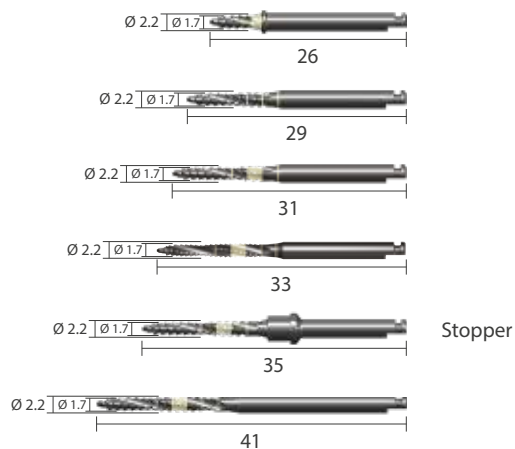

Second Guide Drill

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.6 | 26 | XLD 26 07 |
| | 29 | XLD 26 29 |
| | 31 | XLD 26 31 |
| | 33 | XLD 26 33 |
| | 35 | XLD 26 35 |
| | 41 | XLD 26 41 |

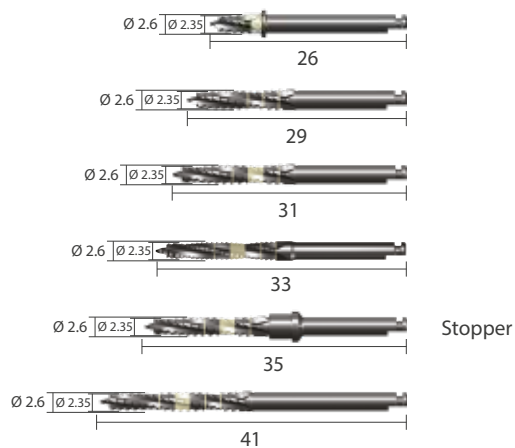


※ Note: Drill speed 1,000rpm, 30~45 N-cm with irrigation


Surgical Instruments

Unit: mm, Scale 1 : 1


Final Drill




| Diameter | L | Art. No. |
|----------|----|--------------|
| Ø 2.9 | 29 | XFD 34 29 |
| Ø 3.35 | | XFD 38 29 |
| Ø 3.85 | | XFD 43 29 |
| Ø 4.4 | | XFD 48 29 |
| Ø 5.4 | | XFD 58 29 SW |




Final Drill



| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.9 | 31 | XFD 34 31 |
| Ø 3.35 | | XFD 38 31 |
| Ø 3.85 | | XFD 43 31 |
| Ø 4.4 | | XFD 48 31 |
| Ø 5.4 | | XFD 58 31 |

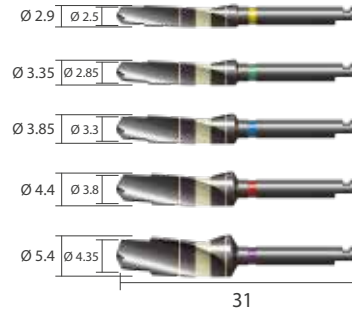

Final Drill




| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.9 | 33 | XFD 34 33 |
| Ø 3.35 | | XFD 38 33 |
| Ø 3.85 | | XFD 43 33 |
| Ø 4.4 | | XFD 48 33 |




※ Note: Drill speed 1,000rpm, 30~45 N-cm with irrigation


Surgical Instruments

Unit: mm, Scale 1 : 1


Final Drill | Stopper 

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.9 | 35 | XFD 34 35 |
| Ø 3.35 | | XFD 38 35 |
| Ø 3.85 | | XFD 43 35 |
| Ø 4.4 | | XFD 48 35 |

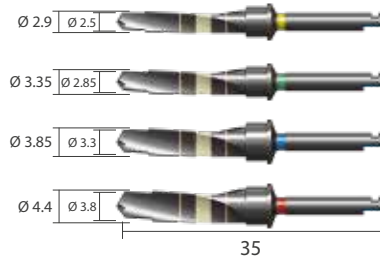

Final Drill 

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.9 | 41 | XFD 34 41 |
| Ø 3.35 | | XFD 38 41 |
| Ø 3.85 | | XFD 43 41 |
| Ø 4.4 | | XFD 48 41 |

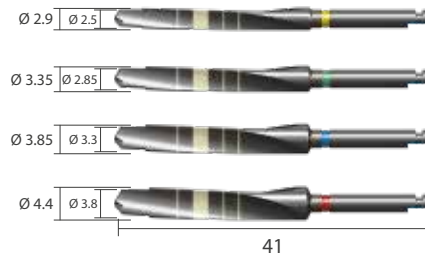

Harvest Drill | Stopper 

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.85 | 35 | XFH 34 35 |
| Ø 3.3 | | XFH 38 35 |
| Ø 3.85 | | XFH 43 35 |
| Ø 4.4 | | XFH 48 35 |



Final Drill | For Short Implant 

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 3.6 | 27 | XFC 36 07 |
| Ø 4.0 | | XFC 40 07 |
| Ø 4.5 | | XFC 45 07 |
| Ø 5.0 | | XFC 50 07 |
| Ø 6.0 | | XFC 60 07 |
| Ø 7.0 | | XFC 70 07 |




Surgical Instruments

Unit: mm, Scale 1 : 1


First | Stopper Drill

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.20 | 8 | XLD 2208S |
| | 10 | XLD 2210S |
| | 12 | XLD 2212S |
| | 14 | XLD 2214S |

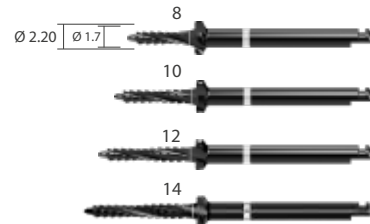


Second | Stopper Drill

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.60 | 8 | XLD 2608S |
| | 10 | XLD 2610S |
| | 12 | XLD 2612S |
| | 14 | XLD 2614S |

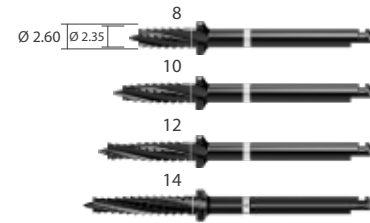

Final | Stopper Drill

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 3.10 | 8 | XFD 3408S |
| | 10 | XFD 3410S |
| | 12 | XFD 3412S |
| | 14 | XFD 3414S |

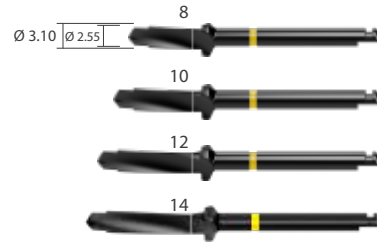

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 3.55 | 8 | XFD 3808S |
| | 10 | XFD 3810S |
| | 12 | XFD 3812S |
| | 14 | XFD 3814S |



| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 3.95 | 8 | XFD 4308S |
| | 10 | XFD 4310S |
| | 12 | XFD 4312S |
| | 14 | XFD 4314S |



| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 4.50 | 8 | XFD 4808S |
| | 10 | XFD 4810S |
| | 12 | XFD 4812S |
| | 14 | XFD 4814S |



※ Note: Drill speed 1,000rpm, 30~45 N·cm with irrigation


Surgical Instruments

Unit: mm, Scale 1 : 1

Countersink




| Diameter | L | Art. No. |
|----------|----|--------------|
| Ø 3.6 | 29 | XCS 36 29 SW |
| Ø 4.0 | 29 | XCS 40 29 SW |
| Ø 4.5 | 29 | XCS 45 29 SW |
| Ø 5.0 | 29 | XCS 50 29 SW |
| Ø 6.0 | 27 | XCS 60 29 SW |
| Ø 7.0 | 27 | XCS 70 29 SW |

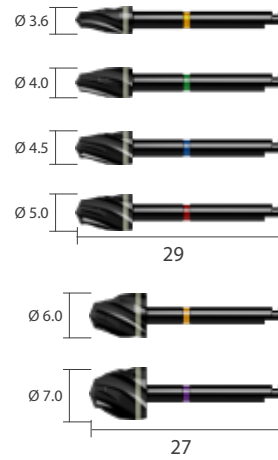

Round Bur

| Diameter | L | Art. No. |
|----------|----|-----------|
| Ø 2.0 | 33 | XRБ 20 33 |
| Ø 3.0 | | XRБ 30 33 |




※ Note: Countersink Drill & Round Bur speed 1,000rpm, 30~45 N·cm with irrigation

Surgical Instruments

Unit: mm, Scale 1 : 1


Stopper I For first guide drill, second guide drill

| Diameter | Drilling Depth | L | Art. No. |
|----------|----------------|------|----------|
| Ø 4.45 | 14 | 4.6 | XLDST 14 |
| | 12 | 6.6 | XLDST 12 |
| | 10 | 8.6 | XLDST 10 |
| | 08 | 10.6 | XLDST 08 |
| | 06 | 12.6 | XLDST 06 |
| | 04 | 14.6 | XLDST 04 |
| | 02 | 16.6 | XLDST 02 |

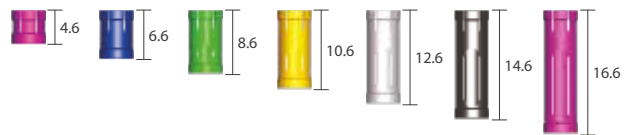


Stopper I For final drill 3435, 3835

| Diameter | Drilling Depth | L | Art. No. |
|----------|----------------|------|----------|
| Ø 5.14 | 14 | 4.6 | XFDST 14 |
| | 12 | 6.6 | XFDST 12 |
| | 10 | 8.6 | XFDST 10 |
| | 08 | 10.6 | XFDST 08 |
| | 06 | 12.6 | XFDST 06 |
| | 04 | 14.6 | XFDST 04 |
| | 02 | 16.6 | XFDST 02 |

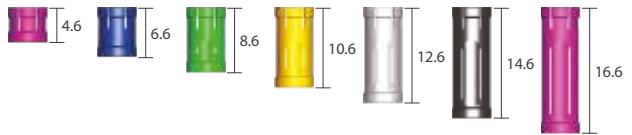

Stopper I For final drill 4335, 4835

| Diameter | Drilling Depth | L | Art. No. |
|----------|----------------|------|------------|
| Ø 5.14 | 14 | 4.6 | XFDST 14 L |
| | 12 | 6.6 | XFDST 12 L |
| | 10 | 8.6 | XFDST 10 L |
| | 08 | 10.6 | XFDST 08 L |
| | 06 | 12.6 | XFDST 06 L |
| | 04 | 14.6 | XFDST 04 L |
| | 02 | 16.6 | XFDST 02 L |


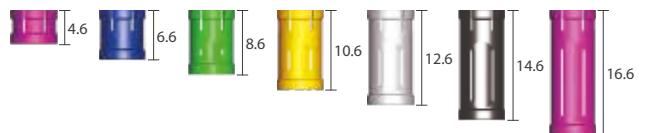


Surgical Instruments

Unit: mm, Scale 1 : 1


Fixture Adapter | Hex 2.5mm

| Type | L | Art. No. |
|------------|----|----------|
| Hand-piece | 27 | XFA 27 H |
| | 30 | XFA 30 H |
| | 32 | XFA 32 H |
| Ratchet | 24 | XFA 24 W |
| | 26 | XFA 26 W |
| | 29 | XFA 29 W |
| | 32 | XFA 32 W |




Fixtrue Adapter-clip | Hex 2.5mm

| Type | L | Art. No. |
|------------|----|----------|
| Hand-piece | 27 | XCA 27 H |
| | 30 | XCA 30 H |
| | 32 | XCA 32 H |
| Ratchet | 24 | XCA 24 W |
| | 26 | XCA 26 W |
| | 29 | XCA 29 W |
| | 32 | XCA 32 W |




Parallel Pin | For first guide drill, second guide drill

| Diameter | L | Art. No. |
|----------|------|--------------|
| Ø 1.6 | 15.5 | XPP 162212 |
| | 20 | XPP 162220 T |
| | 26 | XPP 162226 T |



Path Pin

| Diameter | L | Art. No. |
|----------|------|----------|
| Ø 1.6 | 18.6 | XMFP A 2 |




Surgical Instruments

Unit: mm, Scale 1 : 1



Slot Driver

| Type | L | Art. No. |
|---------|----|----------|
| Ratchet | 17 | SDA 17 R |
| | 25 | SDA 25 R |





Hex Driver | Hex 1.28mm

| Type | L | Art. No. |
|------------|----|-----------|
| Hand-piece | 17 | XHDD 17 H |
| | 25 | XHDD 25 H |
| | 30 | XHDD 30 H |
| Ratchet | 21 | XHD 21 W |
| | 25 | XHD 25 W |
| | 27 | XHD 27 W |
| Manual | 26 | XHD 26 T |
| | 30 | XHD 30 T |




Angled Hex Driver

| Type | L | Art. No. |
|------------|----|----------|
| Hand-piece | 25 | XAD 25 H |
| Ratchet | 21 | XAD 21 W |
| | 25 | XAD 25 W |
| | 27 | XAD 27 W |
| Manual | 26 | XAD 26 T |
| | 30 | XAD 30 T |




Drill Extension

| Diameter | L | Art. No. |
|----------|----|----------|
| Ø 3.0 | 26 | XDE |



Adapter

| Type | Diameter | Art. No. |
|--------|----------|----------|
| Manual | Ø 12.0 | XHDHT |




Surgical Instruments

Unit: mm, Scale 1 : 1

Screw Abutment Adapter

| Type | L | Art. No. |
|------------|----|----------|
| Hand-piece | 20 | XMAA 1 |
| Ratchet | 21 | XMA 21 W |



Mini Ball Abutment Adapter

| Type | L | Art. No. |
|---------|----|-----------|
| Ratchet | 21 | IPST 21 W |



Ratchet

Scale 0.7 : 1

| |
|--------|
| XRCA 1 |
|--------|



Torque Wrench

Scale 0.7 : 1

| |
|------|
| XNTW |
|------|



Depth Gauge

Scale 0.7 : 1


| |
|------|
| XDGL |
|------|

※ Note: One side of Depth Gauge measures the osteotomy depth and the other side measures the gingival height from the top of the implant.



Tissue Punch

| Diameter | L | Art. No. |
|----------|----|----------|
| Ø 4.0 | 27 | XTS 40 |



Osteotome Kit


Unit: mm, Scale 1 : 1

Osteotome

Osteotome compresses the bone laterally, providing denser bony interface rather than removing valuable bone from the surgical site.




Osteotome Kit

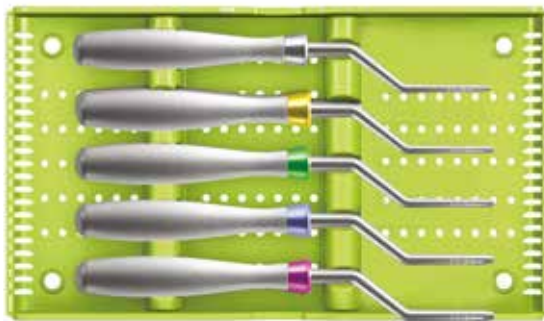

| XOFK | | XOFBK | |
|-----------------|--|------------------|--|
| Type A (Convex) | | Type B (Concave) | |
| XOF 20 A1 | | XOF 20 B1 | |
| XOF 34 A1 | | XOF 34 B1 | |
| XOF 38 A1 | | XOF 38 B1 | |
| XOF 43 A1 | | XOF 43 B1 | |
| XOF 48 A1 | | XOF 48 B1 | |

Osteotome | Final drill type | Scale 0.4 : 1

| Type | Ø A | Ø B | Art. No. |
|----------------------------|-------|-------|-----------|
| Type A (Convex) | Ø 1.7 | Ø 2.8 | XOF 20 A1 |
| | Ø 2.3 | Ø 2.8 | XOF 34 A1 |
| | Ø 2.7 | Ø 3.2 | XOF 38 A1 |
| | Ø 2.8 | Ø 3.8 | XOF 43 A1 |
| | Ø 3.0 | Ø 4.3 | XOF 48 A1 |
| Type B (Concave) | Ø 1.7 | Ø 2.8 | XOF 20 B1 |
| | Ø 2.3 | Ø 2.8 | XOF 34 B1 |
| | Ø 2.7 | Ø 3.2 | XOF 38 B1 |
| | Ø 2.8 | Ø 3.8 | XOF 43 B1 |
| | Ø 3.0 | Ø 4.3 | XOF 48 B1 |

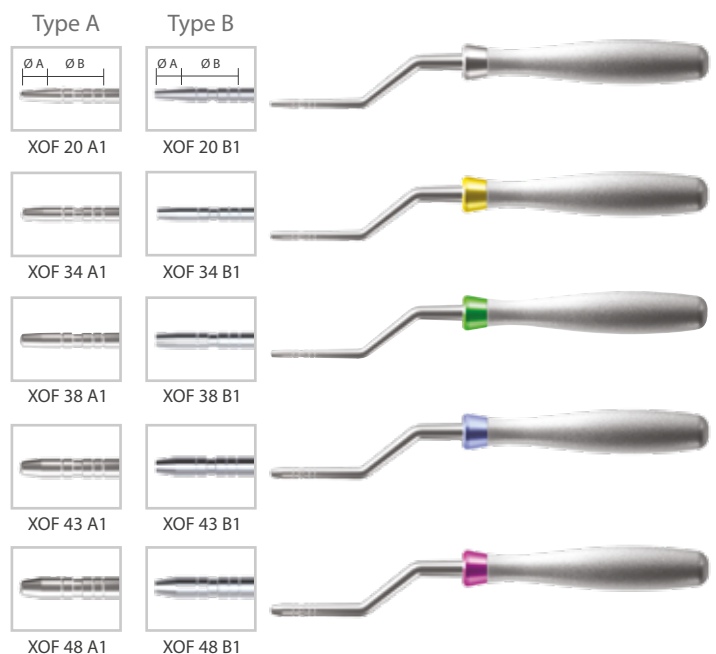


Trephine Kit

Unit: mm, Scale 1 : 1

Trephine Bur

- Excellent fine cutting
- Strong engagement when attaching the trephine to cortical bone
- Cut-outs facilitates ease of harvest retrieval
- 5 scale marks on the Trephine drill from 2mm to 10mm
- Easy harvesting



Trephine Kit




XIT

Kit Includes

| | | | |
|-----------|-----------|-----------|-----------|
| XTP 24 03 | XTP 34 04 | XTP 44 05 | XTP 54 06 |
| XTP 64 07 | XTP 74 08 | XTP 84 09 | XTP 94 10 |

Trephine Bur

| Outer Diameter | Inner Diameter | Art. No. |
|----------------|----------------|-----------|
| Ø 3.0 | Ø 2.4 | XTP 24 03 |
| Ø 4.0 | Ø 3.4 | XTP 34 04 |
| Ø 5.0 | Ø 4.4 | XTP 44 05 |
| Ø 6.0 | Ø 5.4 | XTP 54 06 |
| Ø 7.0 | Ø 6.4 | XTP 64 07 |
| Ø 8.0 | Ø 7.4 | XTP 74 08 |
| Ø 9.0 | Ø 8.4 | XTP 84 09 |
| Ø 10.0 | Ø 9.4 | XTP 94 10 |

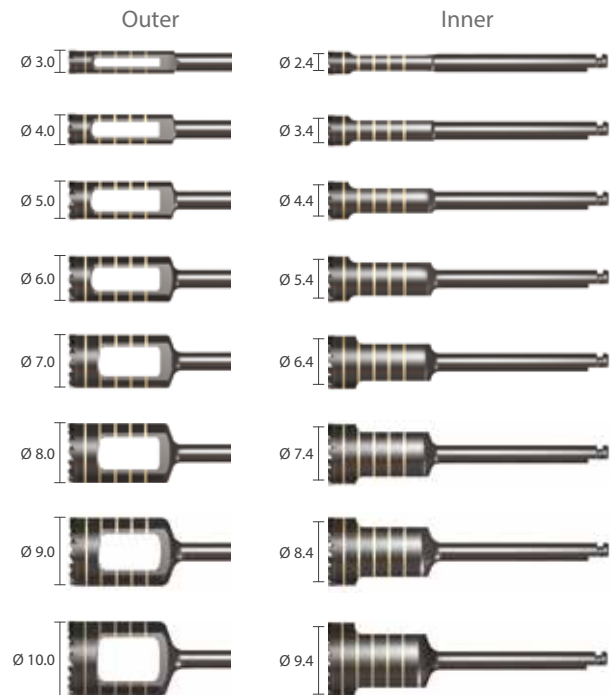


Instrument

Unit: mm, Scale 1 : 1.5

Screw Drill

| Diameter | Art. No. |
|----------|----------|
| Ø1.2 | GMD 1228 |



Membrane screw insertion tool

[Unit: mm, Scale 1 : 0.7]

| Art. No. |
|----------|
| GST26H |
| GST56 |
| GST85 |
| COD |



GST **26H**



GST **56**




GST **85**




COD

Membrane Screws

Unit: mm, Scale 1 : 2

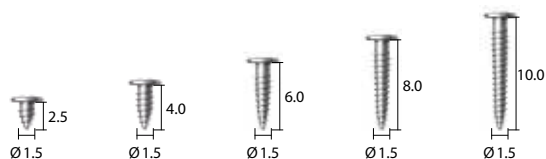


| L | Art. No. |
|------|-----------|
| 2.5 | GSC 15 02 |
| 4.0 | GSC 15 04 |
| 6.0 | GSC 15 06 |
| 8.0 | GSC 15 08 |
| 10.0 | GSC 15 10 |




Screw case | Screw 10ea included

Membrane Pins

Unit: mm, Scale 1 : 2



| L | Art. No. |
|-----|----------|
| 2.8 | GMT3225 |
| 4.5 | GMT3245 |



Pin case | Pin 10ea included




| L | Art. No. |
|-------|----------|
| 125.0 | GMNT |



Membrane Pin with insertion tool

Prosthetic Kit

Unit: mm, Scale 1 : 1

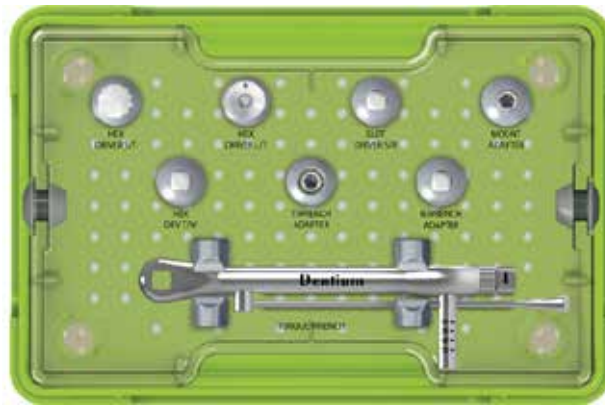

XIP


Hex Driver

| Type | L | Art. No. |
|---------------|----|----------|
| S/T | 15 | XHD 15 |
| L/T | 30 | XHD 30 T |
| Torque Wrench | 25 | XHD 25 W |



Adapter

| Type | L | Art. No. |
|----------------|----|-----------|
| Screw Abutment | 21 | XMA 21 W |
| | 20 | XMAA 1 |
| Mini Ball | 21 | IPST 21 W |

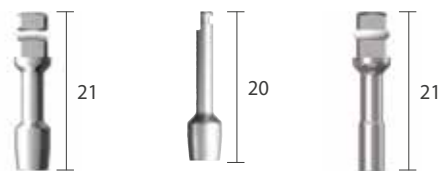

Slot Driver

| |
|----------|
| SDA 25 R |
|----------|




Torque Wrench

| | |
|------|---------------|
| XNTW | Scale 0.7 : 1 |
|------|---------------|



Planning Kit




Unit: mm, Scale 1 : 1

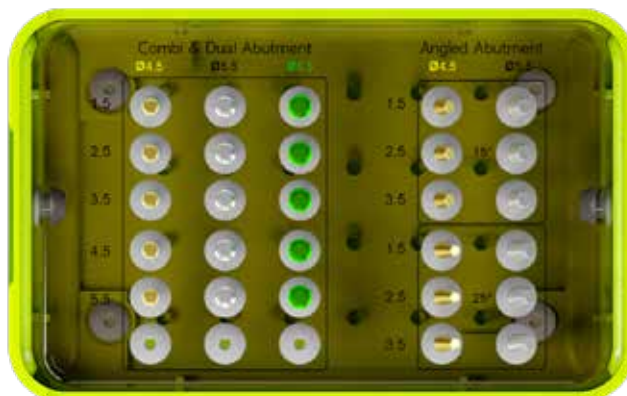

XPX

For Combi & Dual Abutment

| Diameter | G/H | Art. No. |
|----------|-----|-----------|
| Ø 4.5 | 1.5 | PCD 45 15 |
| | 2.5 | PCD 45 25 |
| | 3.5 | PCD 45 35 |
| | 4.5 | PCD 45 45 |
| | 5.5 | PCD 45 55 |
| Ø 5.5 | 1.5 | PCD 55 15 |
| | 2.5 | PCD 55 25 |
| | 3.5 | PCD 55 35 |
| | 4.5 | PCD 55 45 |
| | 5.5 | PCD 55 55 |
| Ø 6.5 | 1.5 | PCD 65 15 |
| | 2.5 | PCD 65 25 |
| | 3.5 | PCD 65 35 |
| | 4.5 | PCD 65 45 |
| | 5.5 | PCD 65 55 |



For Angled Abutment

| Angled | Diameter | G/H | Art. No. |
|--------|----------|-----|--------------|
| 15° | Ø 4.5 | 1.5 | PCA 15 45 15 |
| | | 2.5 | PCA 15 45 25 |
| | | 3.5 | PCA 15 45 35 |
| | Ø 5.5 | 1.5 | PCA 15 55 15 |
| | | 2.5 | PCA 15 55 25 |
| | | 3.5 | PCA 15 55 35 |
| 25° | Ø 4.5 | 1.5 | PCA 25 45 15 |
| | | 2.5 | PCA 25 45 25 |
| | | 3.5 | PCA 25 45 35 |
| | Ø 5.5 | 1.5 | PCA 25 55 15 |
| | | 2.5 | PCA 25 55 25 |
| | | 3.5 | PCA 25 55 35 |




Prosthetic and Laboratory Instrument

Unit: mm, Scale 1 : 1

Hex Driver


| Hex | L | Art. No. |
|------|----|----------|
| 1.28 | 13 | XHD 13 |
| | 15 | XHD 15 |
| | 21 | XHD 21 |
| | 28 | XHD 28 |

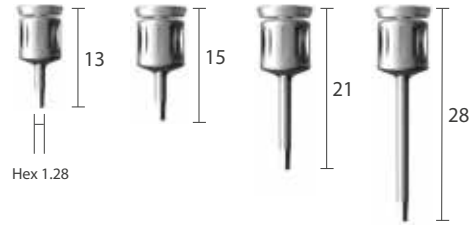

Reamer Guide

| Application | Diameter | Art. No. |
|-----------------------|----------|----------|
| Combi / Dual Abutment | Ø 4.5 | CRG 45 L |
| | Ø 5.5 | CRG 55 L |
| | Ø 6.5 | CRG 65 L |

| Application | Type | Art. No. |
|----------------|--------|----------|
| Screw Abutment | Bridge | SRG BL |
| | Single | SRG SL |

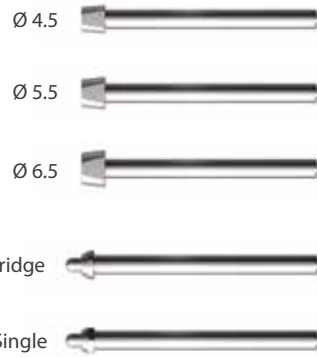

Reamer Handle

Scale 0.5 : 1

| |
|-----|
| CRH |
|-----|



Hand Wrench

| |
|-----|
| XHW |
|-----|




Reamer

| Application | Art. No. |
|-----------------------|----------|
| Combi / Dual Abutment | CRM |
| Screw Abutment | SRM |



Help Kit


Unit: mm, Scale 1 : 1

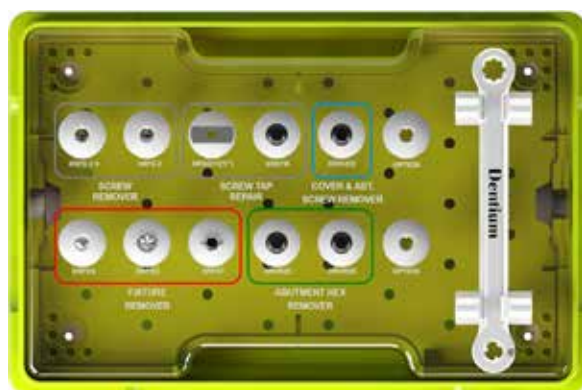

XSHK

Screw Remover

| L | Art. No. |
|----|----------|
| 25 | XRFS 2 S |
| 33 | XRFS 2 |




Screw Tap Repair

| Type | Art. No. |
|-----------|----------|
| Tap | XRSTR |
| 11° Guide | XRSG 11 |




Fixture Remover

| Type | Art. No. |
|---------------|----------|
| Remover Screw | XRFS S |
| Screw Driver | XRFS D |
| Remover | XRFS T |



Abutment Hex Remover

| L | Art. No. |
|----|----------|
| 20 | XRHR 20 |
| 25 | XRHR 25 |



Cover & Abutment Screw Remover

| L | Art. No. |
|----|----------|
| 25 | XRRHDE |



Wrench


Scale 1: 0.7

| |
|-------|
| XRFRW |
|-------|



Polymer Guide Kit


Unit: mm, Scale 1 : 1



PGSSK




PGSCSK

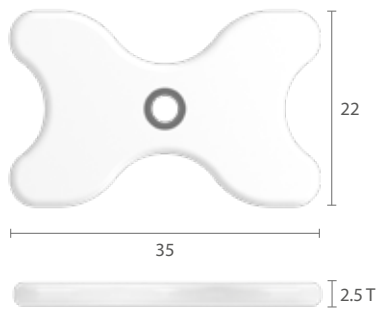

Single Standard (5ea)

| T | Art No. |
|-----|-------------|
| 2.5 | XSG 34 35 S |

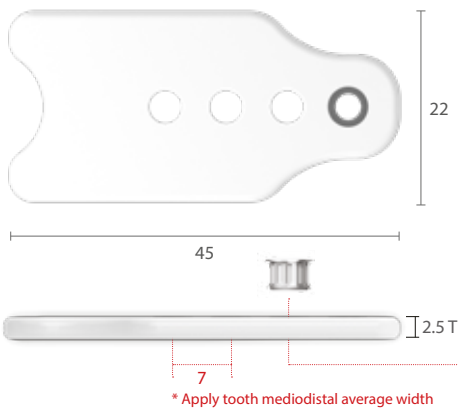

Cantilever Multi-Ready (5ea)

| T | Art No. |
|-----|-------------|
| 2.5 | XSG 34 45 C |

※ 1 fixed Sleeve + 3 additional Sleeve Hole

Stone Drill



XGD 23 60 (1ea)

Guide Pin




XGP 34 23 S (5ea)

Additional Metal Sleeve
(for Cantilever Multi-Ready)



XPGS 34 25 A (5ea)

DASK

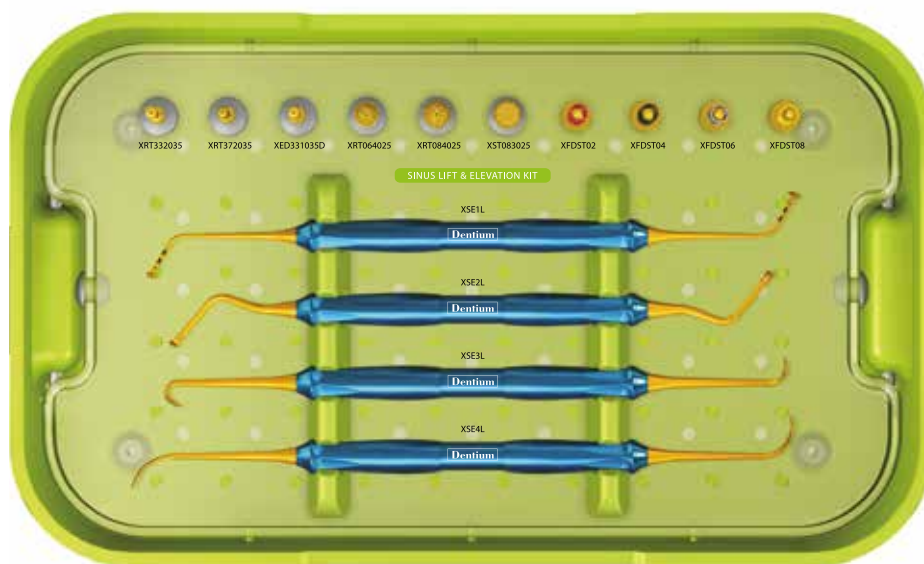

Dentium Advanced Sinus Kit

DASK

Kit Includes

DASK Drill


Stopper



Sinus Elevation Instrument



Sinus Bur Kit

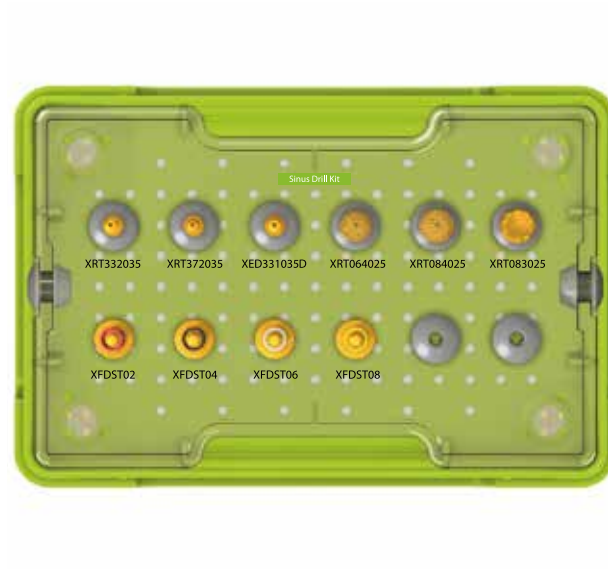

Sinus Bur Kit

SDK

Kit Includes

DASK Drill



Stopper




DASK / Sinus Bur Kit

Unit: mm, Scale 1 : 1

DASK Drill


| Type | DASK Drill # | Art. No. |
|-------------------------|---------------|----------------|
| Crestal Approach | DASK Drill #1 | XRT 33 20 35 |
| | DASK Drill #2 | XRT 37 20 35 |
| | DASK Drill #3 | XED 33 10 35 D |
| Lateral Approach | DASK Drill #4 | XRT 06 40 25 |
| | DASK Drill #5 | XRT 08 40 25 |
| | DASK Drill #6 | XST 08 30 25 |

※ Note: Drill speed 800 to 1,200rpm, 30~45N-cm with irrigation

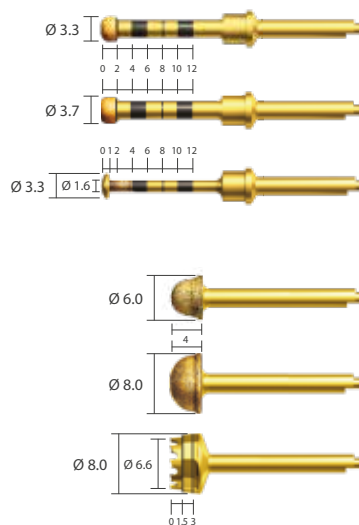


Stopper | For XRT332035, XRT372035, XED331035D


| Diameter | Drilling Depth | L | Art. No. |
|----------|----------------|------|----------|
| Ø 5.14 | 08 | 10.6 | XFDST 08 |
| | 06 | 12.6 | XFDST 06 |
| | 04 | 14.6 | XFDST 04 |
| | 02 | 16.6 | XFDST 02 |



Sinus Elevation Instrument | Scale 0.45 : 1

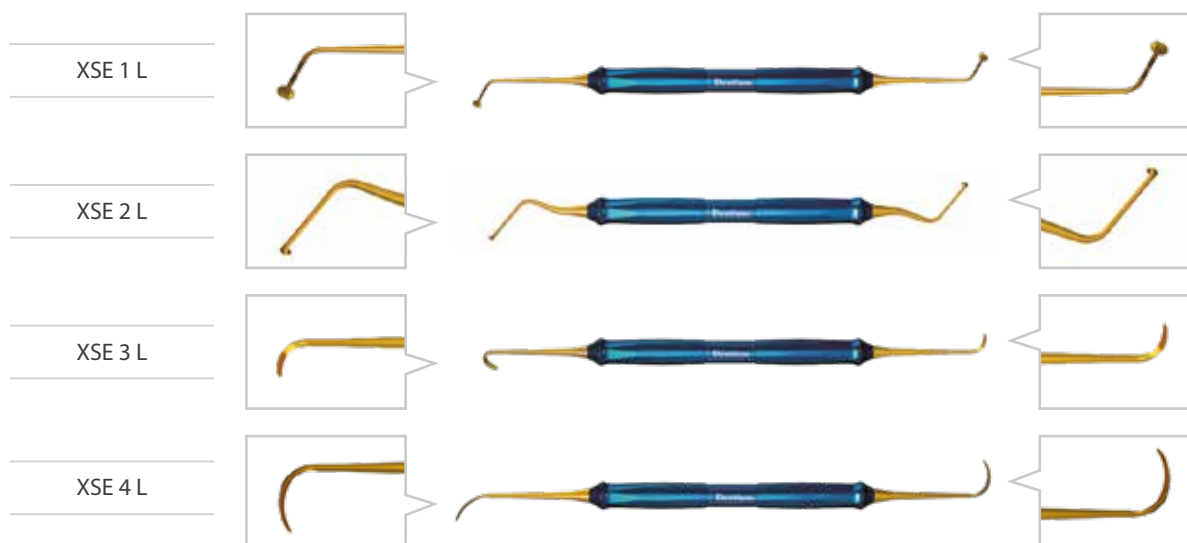

Ridge Spreader Kit

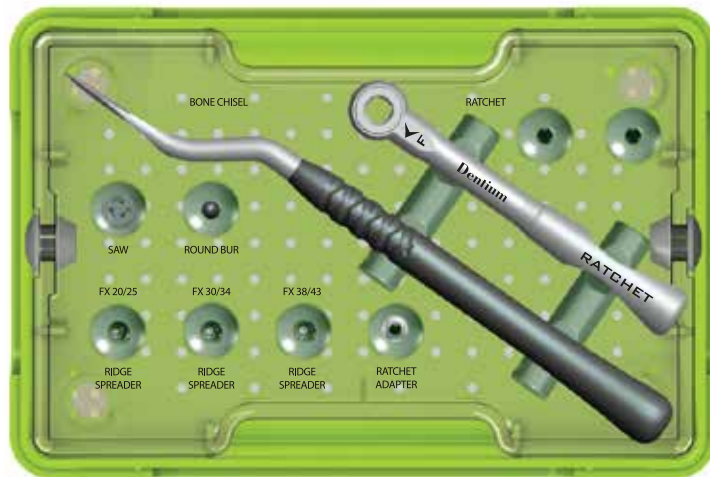

XRSK

Bone Chisel

XBC305013



Ratchet

XRCA1



[Unit: mm, Scale 0.6 : 1]

Ridge Spreader Drills

| Diameter | L | Art No. |
|-------------|----|----------|
| Ø1.4 / Ø2.4 | 35 | RS142435 |
| Ø2.0 / Ø3.2 | 35 | RS203235 |
| Ø2.6 / Ø3.6 | 35 | RS263635 |



Round Bur

| Diameter | L | Art No. |
|----------|----|---------|
| Ø4.0 | 35 | XR4035 |




Ratchet Adapter

XRA3917



Mini Saw


| Diameter | L | Art No. |
|----------|----|---------|
| Ø8.0 | 25 | XDS8025 |



[Unit: mm, Scale 1 : 1]

Sinus Kit

Unit: mm, Scale 1 : 1

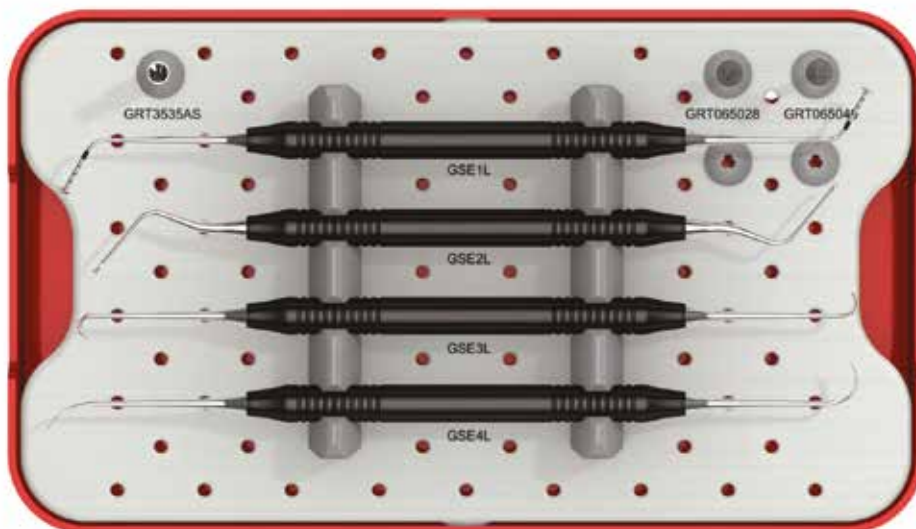


GSEK

Crestal Drill

| Diameter | L | Art No. |
|----------|----|--------------|
| Ø3.5 | 35 | GRT 35 35 AS |


※ Note: Drill speed 20~60 rpm, 30~45N-cm with irrigation



Lateral Drill

| Diameter | L | Art No. |
|----------|----|--------------|
| Ø6.0 | 28 | GRT 06 50 28 |
| Ø6.0 | 40 | GRT 06 50 40 |

※ Note: Drill speed 800 to 1,200rpm, 30~45N-cm with irrigation




Sinus Curette Scale 1 : 2 / mm



Ridge Expander Kit

Unit: mm, Scale 1 : 1

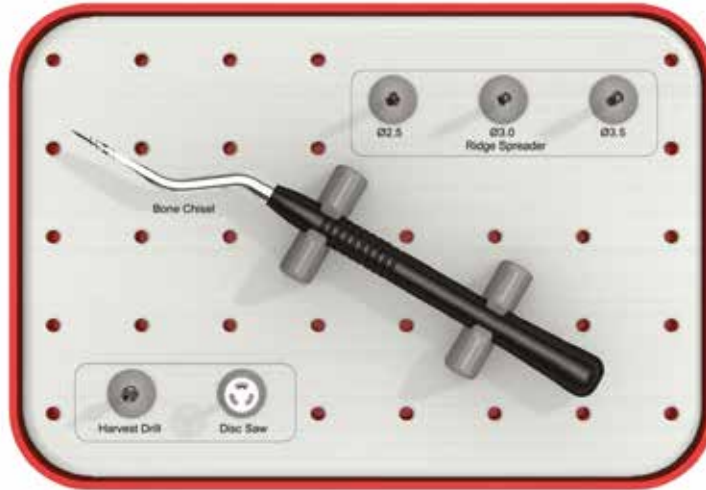


GREK

Ridge Spreader

| Diameter | L | Art No. |
|-------------|----|-----------|
| Ø1.3 / Ø2.5 | 32 | GRS 13 25 |
| Ø1.8 / Ø3.0 | 32 | GRS 18 30 |
| Ø2.3 / Ø3.5 | 32 | GRS 23 35 |

※ Note: condensing drill 20~60 rpm,
30~45N·cm with irrigation



Harvest Drill


| Diameter | L | Art No. |
|----------|----|-----------|
| Ø3.0 | 29 | GHD 30 29 |

※ Note: Harvest Drill speed 20~60rpm,
30~45 N·cm without irrigation



Disc Saw

| Diameter | L | Art No. |
|----------|----|-----------|
| Ø8.0 | 25 | GDS 80 25 |




Bone Chisel

GBC 18 45 13



Implant Guide Kit


Unit: mm, Scale 1 : 1

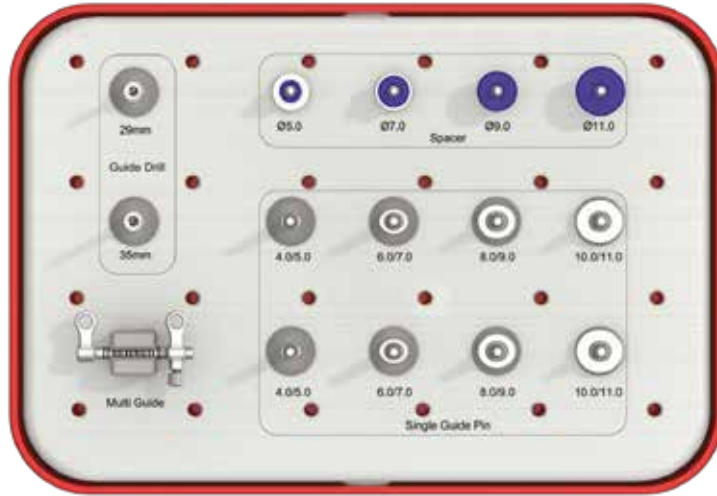

GIGK

Guide Drill

| Diameter | | Art No. |
|----------|----|-----------|
| Ø2.6 | 29 | GGD 26 29 |
| | 35 | GGD 26 35 |




Spacer

| Width | Art No. |
|-------|---------|
| 5.0 | GSP 05 |
| 7.0 | GSP 07 |
| 9.0 | GSP 09 |
| 11.0 | GSP 11 |



Single Guide Pin

| Width | Art No. |
|-------------|-----------|
| 4.0 / 5.0 | GGP 04 05 |
| 6.0 / 7.0 | GGP 06 07 |
| 8.0 / 9.0 | GGP 08 09 |
| 10.0 / 11.0 | GGP 10 11 |

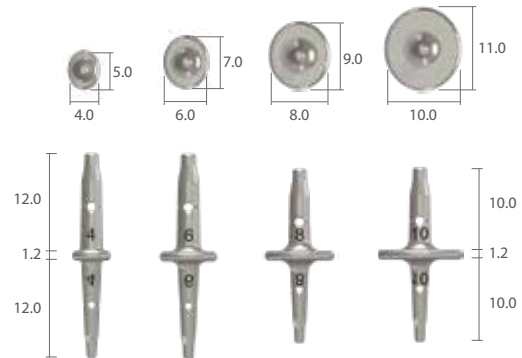


Multi Guide

| |
|------|
| GMG2 |
|------|



Digital Guide | Simple Kit for Positioning, Anchor

Unit: mm, Scale 1 : 1

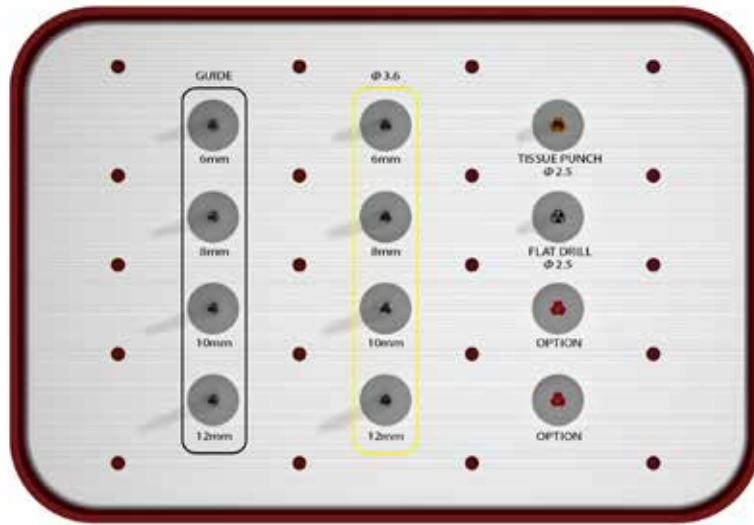


XGSSK

SuperLine FSX3608 Guide Drilling Sequence

| Tissue Punch | Flat Drill | Guide Drill | Final Drill | Adapter |
|--------------|------------|-------------|-----------------|------------------|
| STP25 | SFL25 | SGD2306 | SFD3606 SFD3608 | XCS3629SW XFA30H |

Flapless

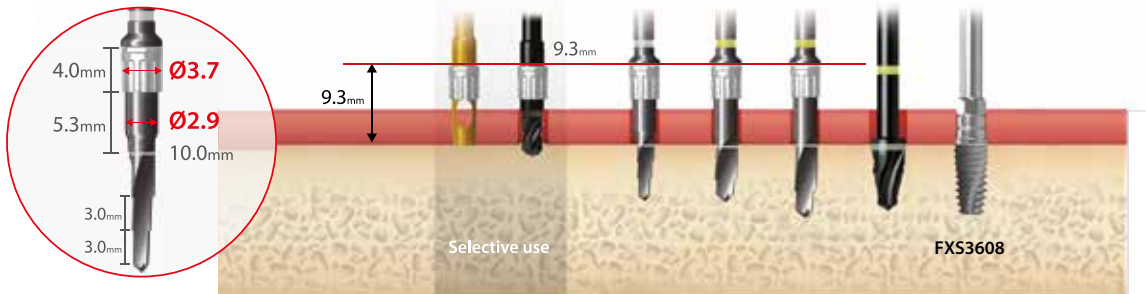


Guide Drill



SGD2306 SGD2308 SGD2310 SGD2312

FX 36 Final Drill



SFD3606 SFD3608 SFD3610 SFD3612

Tissue Punch



STP25

Flat Drill



SFL25

Ti-Sleeve



SMS30


Ti-Open Sleeve



SOS30



Digital Guide | Full Kit for FX 36/40/45

Unit: mm, Scale 1 : 1

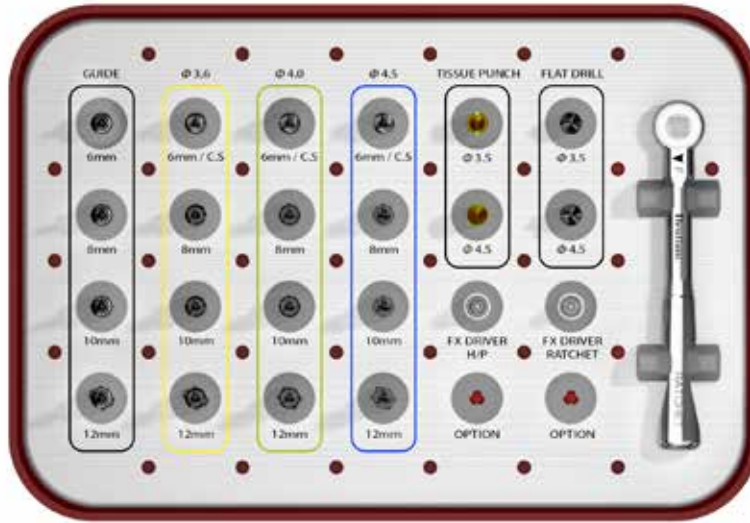


XGSFK

SuperLine FSX4508 Guide Drilling Sequence

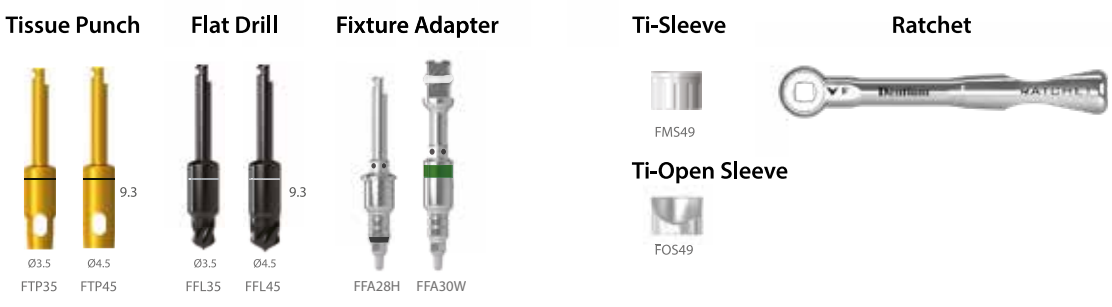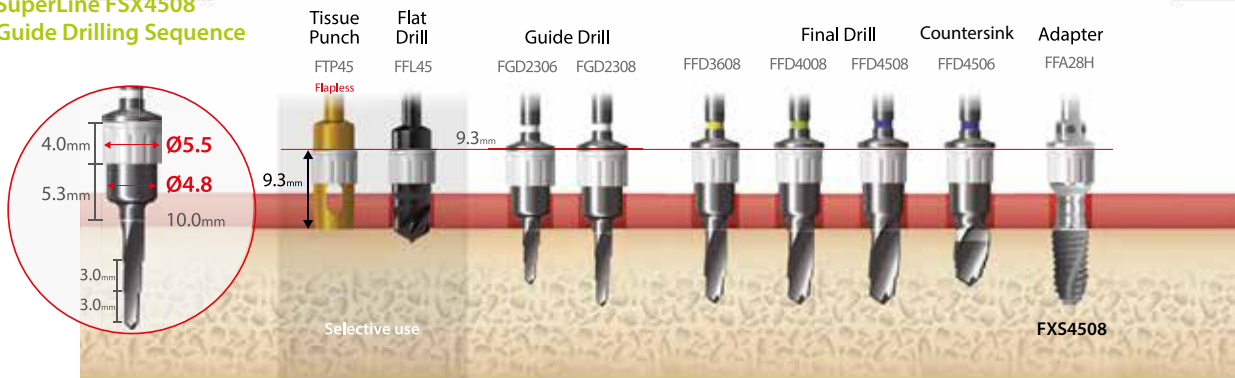


Digital Guide | 5.0 Kit for FX 36/40/45/50

Unit: mm, Scale 1 : 1

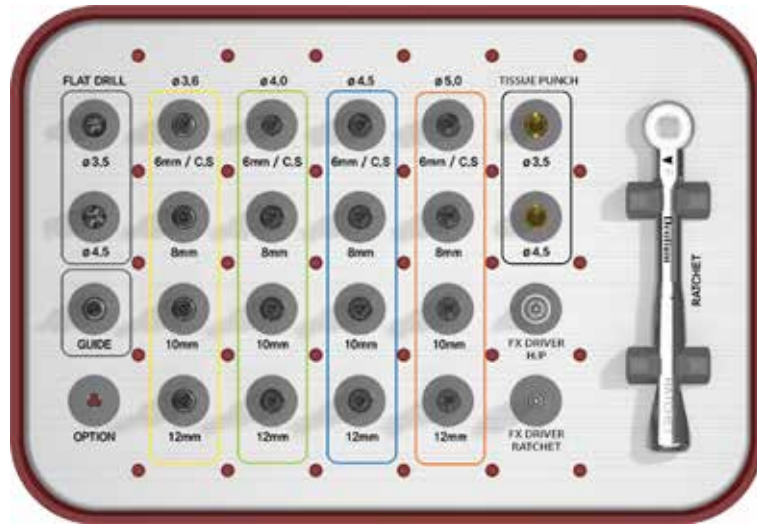

XGSFKW

SuperLine FXS5008 Guide Drilling Sequence

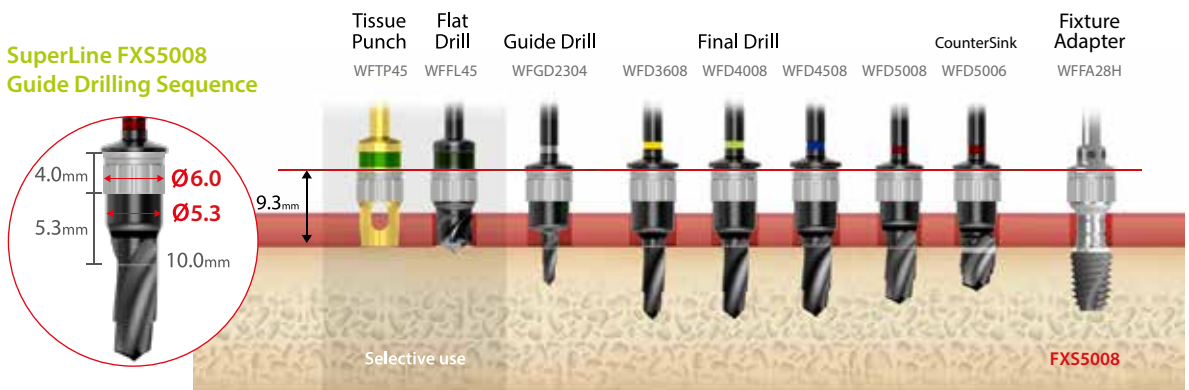

| | | | | |
|---------------------|--|--|--|--|
| Guide Drill | FX36 Final Drill | FX40 Final Drill | FX45 Final Drill | FX50 Final Drill |
| | | | | |
| WFGD2304 | Countersink WFFD3606 WFFD3608 WFFD3610 WFFD3612 | Countersink WFFD4006 WFFD4008 WFFD4010 WFFD4012 | Countersink WFFD4506 WFFD4508 WFFD4510 WFFD4512 | Countersink WFFD5006 WFFD5008 WFFD5010 WFFD5012 |
| Tissue Punch | Flat Drill | Fixture Adapter | Ti-Sleeve | Ratchet |
| | | | | |
| WFTP35 WFTP45 | WFFL35 WFFL45 | WFFA28H WFFA30H | FM554 | XRC1 |
| | | | Ti-Open Sleeve | |
| | | | | |
| | | | FO554 | |

New SuperLine II

Product Catalog

Dentium
For Dentists By Dentists

Specifications are subject to change without any notice.
Some products listed in this catalog are not available in the market due to pending approval.

HEAD OFFICE

174-10, #821 (Gangnam Ace Tower), Jagok-ro, Gangnam-gu, Seoul, Republic of Korea Tel +82-2-555-3750 Fax +82-2-6211-4681

HOME PAGE

www.dentium.co.kr

NS2PC-202101[Rev.0]