

# Description

## Main Configuration:

- **Computer Host:**
- **CPU:** Intel i7 and above, minimum 4 cores, main frequency above 3.2 GHz
- **Memory:** !6 GB or more
- **Hard Disk:** 512 G solid state hard ounce +1 T mechanical hard disk
- **Network card:** 100M or above adaptive, Ethernet 802.3

## Computer Monitor:

- 19 inch or larger monitor screen
- Resolution is 1920x1080 or above

## Operating System:

- Support Windows 7 Professional SP1
- Support Windows 10
- Support Windows Server 2008
- Support Windows Server 2012 R2
- Support HL& Protocol
- 32 bit and 64 bit can run



## Operating System:

- Meets IEC 60950 regulatory requirements for ITE equipment
- Complies with CE's LVD (low voltage) requirements and EMC requirements.
- Computer platform meet the requirements of GB 4943.1-2011, GB17635.1-2012 and GB9254-2008

# Features

## Central Monitoring System

- Supports up to 64 beds or 64 patients across clinical units simultaneously.
- Offers 72-hour storage for 64-channel holographic physiological waveforms.
- Provides review of up to 240 hours of trend data storage and 720 alarm events per bed.
- Historical database enables review of 10,000 discharged patients.
- Supports drug dose calculation and titration table calculation.
- Multiple viewing modes including multiple beds mode, single watch mode, and review mode.
- Supports tabular trends, wave and events, and 12-lead ECG.
- Bi-directional communication with XH-60 Series and XH-80 Series monitors for enhanced patient care.

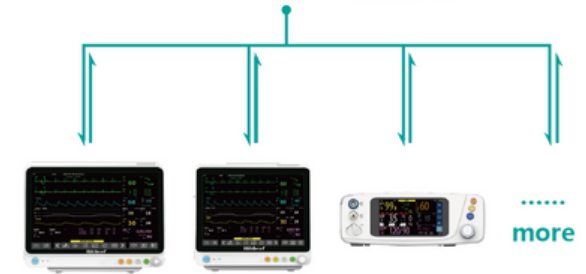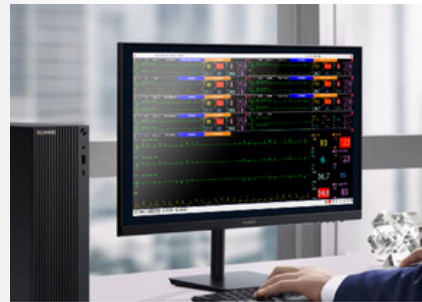

## APS TECHNOLOGY



APS Technology Australia Pty Ltd

APS Technology Australia, Epping,  
NSW, Australia  
info@aps-technology.com.au

